

This document is not an ASTM standard and is intended only to provide the user of an ASTM standard an indication of what changes have been made to the previous version. Because it may not be technically possible to adequately depict all changes accurately, ASTM recommends that users consult prior editions as appropriate. In all cases only the current version of the standard as published by ASTM is to be considered the official document.



Designation: D 5985 – 96^{e1}



Standard Test Method for Pour Point of Petroleum Products (Rotational Method)¹

This standard is issued under the fixed designation D 5985; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

~~¹ Note—Figures A1.1 and A1.2 were editorially corrected in May 1999.~~

INTRODUCTION

This test method covers an alternative procedure for the determination of pour point of petroleum products using an automatic apparatus.

¹ This test method is under the jurisdiction of ASTM Committee ~~D-2~~ D02 on Petroleum Products and Lubricants and is the direct responsibility of Subcommittee D02.07 on Flow Properties.

Current edition approved July Jan. 10, 1996; 2002. Published ~~September 1996~~; March 2002. Originally published as D 5985 – 96. Last previous edition D 5985 – 96^{ε1}.

1. Scope*

1.1 This test method covers the determination of pour point of petroleum products by an automatic instrument that continuously rotates the test specimen against a suspended detection device during cooling of the test specimen.

1.2 This test method ~~includes~~ is designed to cover the range of temperatures from ~~– 57 to + 51°C.~~

~~NOTE 1—The to + 51°C; however, the range of temperatures which were included in the 1992 interlaboratory program only covered the temperature range of – 39 to + 6°C (see 13.4).~~

1.3 This test method determines the no-flow point of petroleum products by detection of the crystal structure or viscosity increase, or both, in the sample that is sufficient to impede flow of the specimen.

1.4 This test method is not intended for use with crude oils.

~~NOTE 1—The applicability of this test method on residual fuel samples has not been verified. For further information on applicability, refer to 13.4.~~

1.5 The values stated in inch-pound units are to be regarded as the standard. The values given in parentheses are for information only.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:

D 97 Test Method for Pour Point of Petroleum Products²

D 4057 Practice for Manual Sampling of Petroleum and Petroleum Products³

D 4177 Practice for Automatic Sampling of Petroleum and Petroleum Products³

2.2 IP Standards:

IP15 Test Method for Pour Point of Petroleum Products⁴

3. Terminology

3.1 Definitions:

3.1.1 *pour point, n—in petroleum products*, the lowest temperature at which movement of the test specimen is observed under prescribed conditions of test.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *no-flow point, n—in petroleum products*, the temperature of the test specimen at which a wax crystal structure or viscosity increase, or both, impedes movement of the surface of the test specimen under the conditions of the test.

² Annual Book of ASTM Standards, Vol 05.01.

³ Annual Book of ASTM Standards, Vol 05.02.

⁴ Available from Institute of Petroleum, 61 New Cavendish St., London, England W1M 8AR.

3.2.2 *Discussion*—The no-flow point occurs when, upon cooling, the formation of wax crystal structures or viscosity increase, or both, have progressed to the point where the applied observation device no longer detects movement under the conditions of the test. The preceding observation temperature, at which flow of the test specimen is last observed, is the pour point.

3.2.3 ~~D 97/IP15 equivalent pour point~~, pour point at 3°C testing intervals, *n*—in petroleum products, the temperature calculated by rounding the no-flow point of the test specimen to the next higher integer which is a multiple of 3°C.

3.2.4 *Discussion*—The no-flow point can be measured with a resolution of 0.1°C in this test method. In Test Method D 97 observations for no-flow are in 3°C intervals and when results with a similar format to Test Method D 97 are required, this calculation shall be performed. Some apparatus can perform this calculation automatically.

3.2.5 *rotational, n*—in this standard, the technique of turning the test specimen jar in an upright position upon a turntable with a stationary positioned, temperature sensor containing pendulum, inserted into the test specimen.

3.2.6 *Discussion*—Upon cooling of the test specimen, the resultant crystal formation or viscosity increase in the specimen exerts force upon the pendulum, offsetting the stationary position and causing detection of the no-flow point.

4. Summary of Test Method

4.1 After inserting the test specimen into the automatic pour point apparatus, and initiation of the program, the test specimen is heated and then cooled by maintaining a constant temperature differential between the cooling block and the sample. The test specimen is continuously tested for flow characteristics by rotating the test specimen cup at approximately 0.1 rpm against a stationary, counter-balanced, sphere-shaped pendulum. The temperature of the test specimen at which a crystal structure or a viscosity increase, or both, within the test specimen causes the displacement of the pendulum is recorded with a resolution of 0.1°C. The test specimen is then heated to the original starting temperature.

5. Significance and Use

5.1 The pour point of a petroleum product is an index of the lowest temperature of its utility for certain applications. Flow characteristics, such as pour point, can be critical for the correct operation of lubricating systems, fuel systems, and pipeline operations.

5.2 Petroleum blending operations require precise measurement of the pour point.

5.3 This test method can determine the temperature of the test specimen with a resolution of 0.1°C at which either crystals have formed or viscosity increases sufficiently to impede movement of the petroleum product.

5.4 This test method yields a ~~D 97/IP15 equivalent pour point~~ in a format similar to Test Method D 97/IP15 when the 3°C interval results are reported.

NOTE 2—Since some users may wish to report their results in a format similar to Test Method D 97 (in 3°C intervals) the precisions were derived for the temperatures rounded to the 3°C intervals. ~~The term equivalent is intended to mean in the same format.~~ For statements on bias relative to Test Method D 97, see 13.3.

5.5 This test method has better repeatability and comparable reproducibility relative to Test Method D 97 as measured in the 1992 interlaboratory program.⁵

6. Apparatus

6.1 *Automatic Apparatus*⁶—The automatic pour point apparatus described in the Annex A1 consists of a microprocessor controlled measuring unit that is capable of heating, cooling, rotating, and recording the temperature of the test specimen. The apparatus shall be equipped with a digital display, cooling/heating block assembly, turntable, test specimen cup and measuring head containing a counter-balanced pendulum and temperature measuring device.

6.2 *Test Specimen Cup*—The test specimen cup is a flat bottom aluminum cup with the dimensions in A1.2. To indicate the required fill level, the inside of the test cup is scribed at a height of 36 ± 0.2 mm above the inside bottom. The outside bottom of the test cup has two indentions to facilitate the rotation of the test cup.

6.3 *Circulating Bath*—Refrigeration unit equipped with a circulating pump capable of maintaining a temperature at least 20°C colder than the lowest expected pour point to be measured.

7. Reagents and Material

7.1 *Methyl Alcohol*, anhydrous, for use as cooling medium in circulating bath.

7.2 *Cleaning Solvents*, suitable for cleaning and drying the specimen cup and pendulum, such as petroleum naphtha and ~~acetone~~.

NOTE 3—~~Warning: Flammable: acetone. (Warning—Flammable. Liquid causes eye burns. Vapor harmful. May be fatal or cause blindness if swallowed or inhaled.)~~

8. Sampling

8.1 Obtain a sample in accordance with Practices D 4057 or by D 4177.

⁵ The results of the 1992 Interlaboratory Cooperative Test Program are available from ASTM International Headquarters in the form of a research report. Request RR:D02-1312.

⁶ The following instrument has been found suitable for use in this test method: Herzog Model MC 850 available from Walter Herzog, Lauda, Germany.

8.2 Samples of very viscous materials can be warmed until they are reasonably fluid before they are transferred; however, no sample shall be heated more than is absolutely necessary. The sample shall not be heated and transferred into the test specimen cup unless its temperature is 70°C or lower.

NOTE 4~~3~~—In the event the sample has been heated above this temperature, allow the sample to cool until its temperature is at least 70°C before transferring.

9. Preparation of Apparatus

9.1 Prepare the instrument for operation in accordance with the manufacturer's instructions.

9.2 Clean and dry the test specimen cup and the cooling well using suitable solvents as prescribed by the apparatus manufacturer.

9.3 Prepare the refrigerated circulating bath for operation in accordance with the manufacturer's instructions and allow it to attain a temperature at least 20°C lower than the expected pour point of the sample.

10. Calibration and Standardization

10.1 Ensure that all of the manufacturer's instructions for calibrating, checking, and operating the apparatus are followed.

10.2 Adjust the position of the measuring pendulum, when necessary, according to the manufacturer's instructions.

10.3 A sample with a well documented pour point can be used to verify performance of the apparatus. Alternatively, a sample which has been extensively tested in a pour point interlaboratory study can be used.

11. Procedure

11.1 Transfer the specimen into the test specimen cup to the scribed mark. When necessary, heat the sample in a water bath or oven until it is just sufficiently fluid to transfer into the test specimen cup. Samples with an expected pour point above 36°C or which appear solid at room temperature can be heated above 45°C but shall not be heated above 70°C (see Note 4~~3~~).

~~11.2 Samples of residual fuels, black oils, and cylinder stock, which 3).~~

NOTE 4—Residual fuels have been heated known to a temperature higher than 45°C during the preceding 24 h or when the be sensitive to thermal history of. In the case where a residual fuel sample types is not known, shall be kept at room temperature tested, refer to Test Method D 97 for 24 h before testing.

~~11.3 Make sample treatment.~~

11.2 Make sure that the cooling well is free of moisture. If it is not, remove all moisture by wiping with a dry cloth. Insert the test specimen cup into the cooling well. Bring the measuring head into position over the test specimen cup and lower it into the test specimen.

~~11.43 Start the test program following the manufacturer's instructions.~~

11.54 When the expected pour point is known to be higher than -33°C , preselect a starting temperature which is at least 9°C higher than the expected pour point, but at least 45°C. The highest starting temperature that can be programmed is 70°C.

11.65 When the expected pour point is known to be at or below -33°C , the test duration can be shortened by preselecting a starting temperature which is at least 9°C higher than the expected pour point. The lowest starting temperature that can be programmed is 20°C.

11.76 When the expected pour point is not known and the sample appears to be liquid, preselect a starting temperature of 45°C. The apparatus automatically heats the test specimen to approximately 45°C when a starting temperature is not selected. When the expected pour point is not known and the sample needs to be heated before transferring into the test specimen cup, preselect a starting temperature of 70°C.

11.87 Initially, the test specimen is heated to approximately 45°C, or to the starting temperature preselected by the operator between 20 and 70°C. The test specimen cup is continuously rotated at approximately 0.1 rpm and flow of the cooling fluid from the circulating bath is regulated to maintain the cooling block at a temperature approximately 8°C lower than the test specimen temperature. The test specimen temperature is continuously displayed. At the detection of the last flow point, the temperature the test specimen attained is held on the digital display until reset by the operator. The test specimen is then heated to approximately 45°C, or to the preselected temperature.

11.98 The test specimen temperature rounded up to the next 3°C integer is also displayed.

12. Report

12.1 Report the temperature recorded in 11.87, with resolution of 0.1°C, as the no-flow point in accordance with Test Method D 5985 (rotational method).

12.2 Report the temperature recorded in 11.98 as the ~~D 97 equivalent~~ pour point at 3°C testing intervals in accordance with Test Method D 5985.

13. Precision and Bias

13.1 Precision—The precision of this test method as determined by the statistical examination of the interlaboratory test results is as follows:⁶

13.1.1 ~~D 97 Equivalent~~ *Pour Point at 3°C Testing Intervals (Rotational Method)*:

13.1.1.1 *Repeatability*—The difference between successive test results, obtained by the same operator using the same apparatus under constant operating conditions on identical test material, would in the long run, in the normal and correct operation of this test method, exceed the following only in one case in twenty.

2.3°C

13.1.1.2 *Reproducibility*—The difference between two single and independent test results, obtained by different operators working in different laboratories on identical test material, would in the long run, in normal and correct operation of this test method, exceed the following only in one case in twenty.

8.7°C

13.1.2 *No-Flow Point—Repeatability*—The difference between successive test results, obtained by the same operator using the same apparatus under constant operating conditions on identical test material, would in the long run, in the normal and correct operation of this test method, exceed the following only in one case in twenty.

1.18°C

13.2 *Bias*—Since there is no accepted reference material suitable for determining the bias for the procedure in this test method, bias has not been determined.

13.3 *Relative Bias*—~~Relative bias⁵ among certain samples, was observed when the D 97/IP15 equivalent pour point results;~~

~~13.3.1 Pour points at 3°C testing intervals were compared to the results from Test Method D 97. The Relative bias⁵ among certain samples was observed; however, the observed bias does not appear to be of a systematic nature and is within the reproducibility of either test method. Bias nature. Biases relative to Test Method D 97/IP15 may conceivably occur for sample types not included in the laboratory test program.~~

~~NOTE 5—Large differences in results were observed between methods for one sample in the Interlaboratory Test Study. The sample was a high-sulfur winter diesel. When cooled during the performance of a new formulation or test method, this sample formed thin, but very large crystals, that could be described as large plates. These crystals formed wherever sample-glass contact was made as well as covered; the performance top surface of the sample. The entire sample, except for this all encasing thin skin of crystals, remained liquid with apparent low viscosity. When this occurred and the sample was handled gently, the sample did not pour, but with rougher handling, the crust broke and the sample poured readily. Users of this method shall be compared are advised to Test Method D 97 before reporting be alert for differences in results as Test Method D 97 equivalent. between test methods when this behavior is observed in the sample being tested.~~

13.4 The precision statements in 13.1.1 were derived from the 1992 interlaboratory test program. Participants analyzed three sets of duplicate fuel oils and six sets of duplicate lubricating oils in the temperature range of + 6 to – 39°C. Six laboratories participated with the automatic apparatus and seven laboratories participated with the manual Test Method D 97 apparatus. Information on the types of samples and their average pour points are in the research report available from ASTM International Headquarters.⁵

13.5 The precision statements in 13.1.2 were derived from the 0.1°C resolution data obtained from two within-one-laboratory test programs. The first program in 1984 consisted of twelve sets of duplicate lubricating oils and fuel oils, and fourteen sets of duplicate fuel oils in the temperature range from + 51 to – 51°C. The second was part of the 1992 interlaboratory program where one laboratory submitted 0.1°C resolution data along with the calculated 3°C results on the same samples. The repeatability is calculated using the program described in RR:D2-1007 on the results obtained from the 1984 program which was the worst case of the two programs. This data does not meet ASTM criteria for RR:D02-1007.

14. Keywords

14.1 D 97 equivalent; petroleum products; pour point; rotational pour point

ANNEX

(Mandatory Information)

A1. POUR POINT APPARATUS

A1.1 *Cooling/Heating Block Assembly*—The test specimen cup is contained within an assembly to facilitate heating, cooling, and rotation of the test specimen cup (see Fig. A1.1). The dimensional requirements are only such that the prescribed rate of cooling and rotation of the test specimen cup shall be maintained. Provision shall be provided for suspension of the pendulum and measurement of the specimen temperature.

A1.2 *Test Specimen Cup*, made of aluminum with the following dimensions: aluminum (see Fig. A1.2).

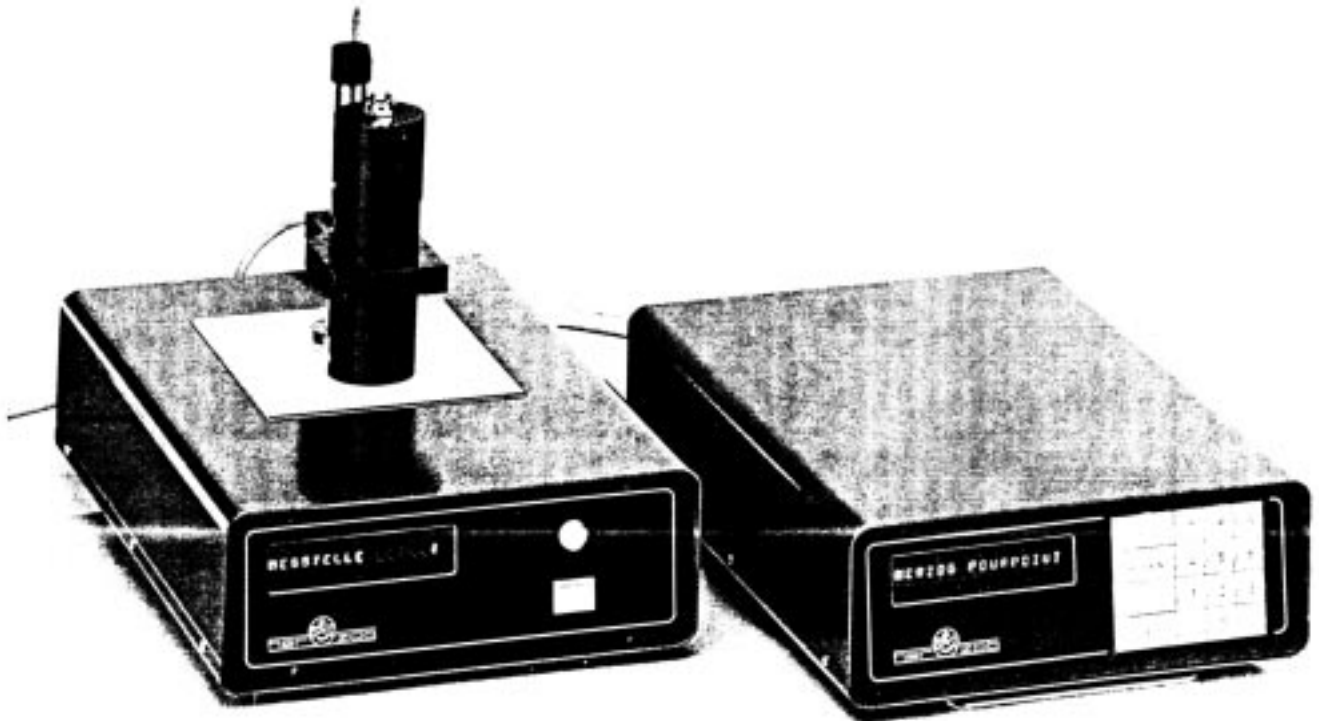


FIG. A1.1 Cooling/Heating Block Assembly

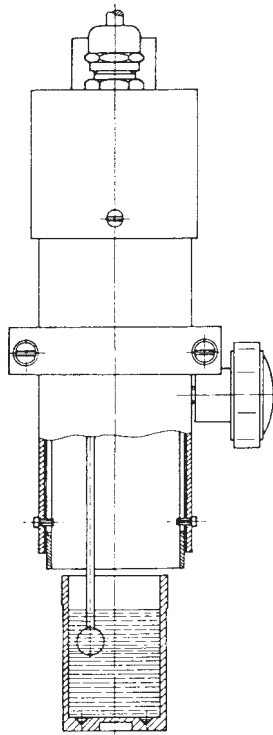


FIG. A1.2 Test Specimen Cup

Outside diameter	36 ± 0.5 mm
Wall thickness	2 ± 0.1 mm
Length	51 ± 0.5 mm
Above inside bottom to locate scribe line	36 ± 0.2 mm

A1.3 Temperature Measuring Device—The temperature measurement can be accomplished through any convenient means such as a platinum resistance device. The resolution of the temperature measurement shall be to 0.1°C and the tolerance of the device shall be less than 1 %.

SUMMARY OF CHANGES

Committee D02 has identified the location of selected changes to this standard since the last issue (D 5985-96^{e1}) that may impact the use of this standard.

(1) Introduction—an Introduction was added similar to Test Methods D 5949 and D 5950, the equivalency relation to Test Method D 97 has been removed, any sections containing this relation are also removed.

(2) Paragraph 1.2—Note 1 is incorporated into this subsection.

(3) Paragraph 11.3—References to residual fuel testing are removed as applicability has not been verified.

(4) Section 13, Precision—the Relative Bias section was changed to be similar in context to the same sections in Test Methods D 5949 and D 5950.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).