

This document is not an ASTM standard and is intended only to provide the user of an ASTM standard an indication of what changes have been made to the previous version. Because it may not be technically possible to adequately depict all changes accurately, ASTM recommends that users consult prior editions as appropriate. In all cases only the current version of the standard as published by ASTM is to be considered the official document.



---

**Designation: D 1054 – 91 (Reapproved 2000)**


**Designation: D 1054 – 02**

# Standard Test Method for Rubber Property—Resilience Using a Goodyear-Healey Rebound Pendulum<sup>1</sup>

This standard is issued under the fixed designation D 1054; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ε) indicates an editorial change since the last revision or reapproval.

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D11 on Rubber and is the direct responsibility of Subcommittee D11.14 on Time and Temperature-Dependent Physical Properties.

Current edition approved ~~March 15, 1994~~; Dec. 10, 2002. Published ~~May 1994~~; January 2003. Originally published as ~~D 1054 – 49F~~; approved in 1949. Last previous edition approved in 2000 as D 1054 – 8791 (2000).

## 1. Scope

1.1 ~~This~~ test methods covers the determination of impact resilience and penetration of rubber by means of the Goodyear-Healey rebound pendulum, see Fig. 1.

1.1.1 The term rubber, used within this method, shall refer to those substances classified as thermoplastic elastomers, vulcanized (thermoset) rubber, elastomeric materials, and cellular materials.

1.2 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only. Many of the stated dimensions in SI are direct conversions from the U.S. Customary System to accommodate the instrumentation, practices and procedures that existed prior to the Metric Conversion Act of 1975.

1.3 All materials, instruments, or equipment used for the determination of mass, force, direction, temperature or dimension shall have traceability to the National Institute for Standards and Technology, or other internationally recognized organization parallel in nature.

1.4 *This standard does not purport to address all of the safety ~~problems, concerns,~~ if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

### 2.1 ASTM Standards:

D 3182 Practice for Rubber—Materials, Equipment, and Procedures for Mixing Standard Compounds and Preparing Standard Vulcanized Sheets<sup>2</sup>

D 3183 Practice for Rubber—Preparation of Pieces for Test Purposes from Products<sup>2</sup>

D 4483 Practice for Determining Precision for Test Method Standards in the Rubber and Carbon Black Industries<sup>2</sup>

E 145 Specification for Gravity—Convection and Forced-Ventilation Ovens<sup>3</sup>

## 3. Summary of Test Method

~~3.1 Test Method A covers the use of the Goodyear-Healey rebound pendulum. See Fig. 1.~~

~~3.2 Test Method B covers the use of the SCHOB rebound pendulum.~~

~~3.3~~

3.1 Impact Resilience—A freely falling pendulum hammer that is dropped from a given height impacts a test specimen and ~~imparts to it specimen, imparting~~ a certain amount of energy; a portion of that energy is returned by the specimen to the pendulum and may be measured by the extent to which the pendulum rebounds. Since the energy of the pendulum is proportional to the vertical component of the displacement of the pendulum, it may be expressed as  $1 - \cos$  (of the angle of displacement) and impact resilience.  $RB$ , is readily determined from the equation.


$$RB = \frac{1 - \cos(\text{angle of rebound})}{1 - \cos(\text{original angle})} \times 100 \quad (1)$$

3.31.1 The value  $RB$  is commonly called percentage rebound.

<sup>2</sup> Annual Book of ASTM Standards, Vol 09.01.

<sup>3</sup> Typical apparatus can be obtained from Zwick

<sup>3</sup> Annual Book of America, L. A. Anderson Co., PO Box 5400, Akron, OH. Request Model 5109.01. ASTM Standards, Vol 14.04.

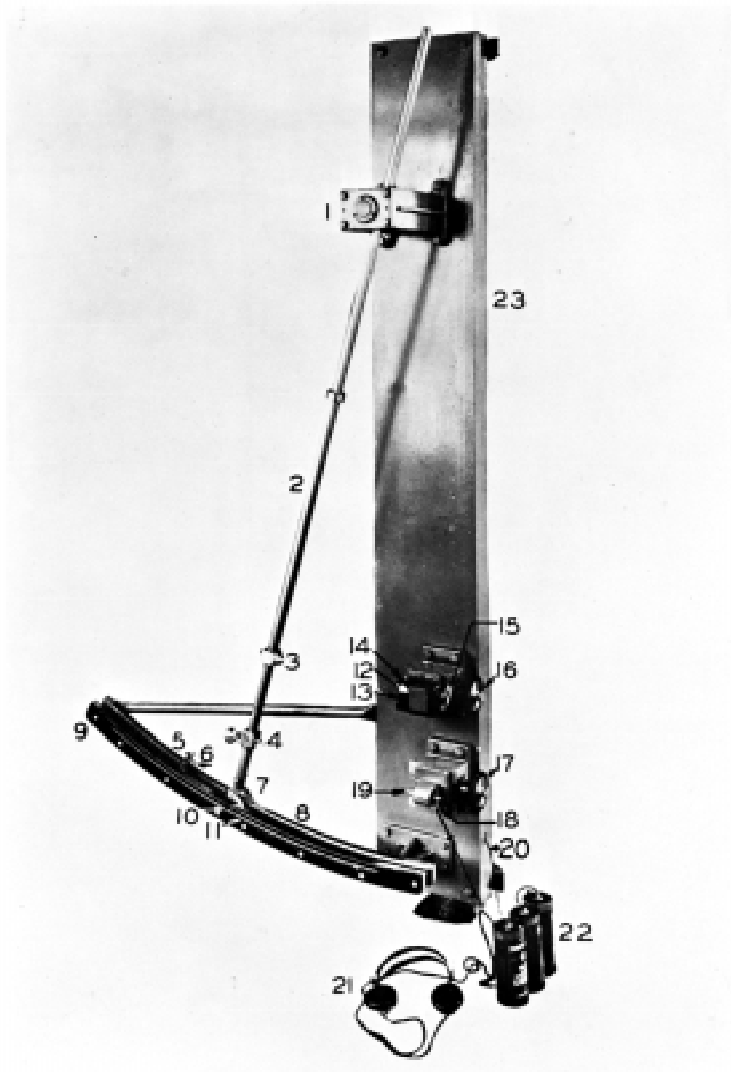

NOTE 1—Except where rough finish is indicated, all surfaces shall be machined to a smooth finish within the dimensions and tolerances indicated. Boiler-plate steel is suitable material.

FIG. 1 Goodyear-Healey Rebound Pendulum

3.42 *Penetration*—Dynamic stiffness is a factor that influences impact resilience. A convenient index of stiffness is the depth to which the pendulum penetration striker penetrates the test specimen upon impact.

3.5 *Rebound Resilience*—The apparatus for indicating the rebound resilience should permit the most friction-free possible measurement of the angle of rebound  $\alpha$ . From the rebound angle  $\alpha$ , the rebound resilience in percent is obtained according to the following formula:

$$R = (1 - \cos \alpha) \cdot ICU \quad (2)$$

#### 4. Significance and Use

4.1 The Goodyear-Healey<sup>4</sup> rebound pendulum is designed to measure percent resilience of a rubber compound as an indication of hysteretic energy loss that can also be defined by the relationship between storage modulus and loss modulus. The percent rebound measured is inversely proportional to the hysteretic loss.

4.2 Deflection is determined by measuring the depth of penetration of the rebound ball into the rubber block under test.

4.3 Percent resilience and deflection are commonly used in quality control testing of polymers and compounding chemicals, especially reinforcing material.

<sup>4</sup> This instrument is no longer available from the Goodyear Tire and Rubber Co., Process Engineering and System Designs, Dept. 109 E, 1144 East Market Street, Akron, OH 44316. Technical and engineering drawings for its manufacture and the reproduction of replacement parts are available from ASTM at a nominal cost. Request Adjunct Number ADJD1054.

5. Apparatus

5.1 Rebound Pendulum— The Goodyear-Healey rebound-resilience is measured with a mechanical vibration device with one degree pendulum (see Fig. 1) shall consist of freedom. Various practical designs of these devices are on the market. Regardless of following:

5.1.1 Ball bearings (1), which support the form, these devices essentially provide pendulum,

5.1.2 Free swinging pendulum (2),

5.1.3 Penetration striker (3),

5.1.4 Contact for the same values of the rebound-resilience if the parameters of the instruments lie within the limits reported in 5.2.5 (Test Method B):

5.2 Description of Apparatus:

5.2.1 The apparatus<sup>5</sup> consists of a frame indentation reading (4),

5.1.5 Release device (5 and 6),

5.1.6 Pawls (7),

5.1.7 Pawl rack (8),

5.1.8 Pointer (10),

5.1.9 Anvil (12),

5.1.10 Quadrant with an anvil, a angular scale (11),

5.1.11 Specimen holder for the specimen, a pendulum with a hammer peen, (14),

5.1.12 Penetration micrometer (16, 17, and 18),

5.1.13 Headphones (21) and a device for indicating the rebound-resilience, see Fig. 2.


5.2.1.1 The frame with anvil together must have a mass that is at least 100 times greater than the striking mass of the pendulum.

5.2.1.2 The holder must ensure a fixed position of the specimen not tapering dry battery circuit (22), or other suitable power supply, attached to the side. The holder should have penetration micrometer for determining when the same effect as that achieved by gluing the specimen to the striking surface. The difference between the rebound-resilience moment of the held specimen compared to that contact of the glued specimen should be less than two units of rebound-resilience. This condition must be satisfied both in contact for the ease of highly elastic specimens (rebound-resilience around 90 %) and in the case of very hard (hardness 80 to 85 IRHD) samples. The holder may be designed as a mechanical clamping device or as a vacuum holder or combination of the two:

5.2.1.3 The indentation reading (4), and

5.1.14 Vertical base (23).

5.2 The steel pendulum consists of a pendulum rod, hammer, and a hammer peen, see Fig. 2. The pendulum is suspended in such a way that under the influence of gravity, it rotates in a planar path. When the pendulum is hanging vertically, the hemispherical hammer peen should just touch the surface of the specimen. The striking direction of the hammer peen must be

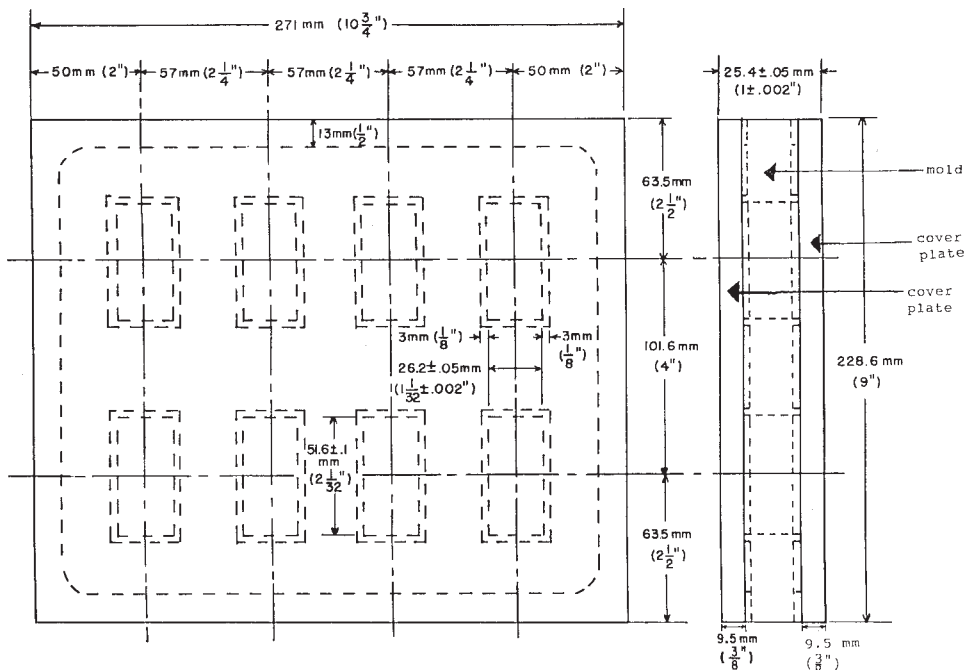

NOTE 1—Dimensions unless otherwise specified are to be  $\pm 0.05$  mm ( $\pm 0.002$  in.).

FIG. 2 Mold for Test Specimens

perpendicular bar (2) shall conform to the specimen surface.

5.2.2 The testing parameters with their tolerances are as follows:  
following dimensions:

Hemisphere diameter,  $D$ ,  
Hemisphere diameter,

	mm	in.
Length of hammer peen:	12.45 to 15.05 mm	
Length of pendulum bar, overall (2)	12.45 to 15.05 mm	
Effective mass of pendulum, $m$ ,	0.247 to 0.35 kg	
Effective mass of pendulum, $m$ , $1825 \pm 2$	$72.80 \pm 0.08$	
Striking velocity, $v$ , and	1.45 to 2.04 m/sec.	
Diameter of pendulum bar (2)	1.45 to 2.04 m/sec.	
Apparent deformation energy density ( $D^*d$ ),	325 to 465 kJ/m	
Apparent deformation energy density ( $D^*d$ ), $23.17 \pm 0.13$	$325$ to $465$ kJ/m	

5.2.3 The original apparatus had the following parameters:

$-0.912 \pm 0.005$	$D = (15.00 \pm 0.05)$ mm
	Diameter of penetration striker (3)
	$22.22 \pm 0.13$

With these parameter values and the specified specimen thickness  $d = 12.50.875 \pm 0.5$  mm, the apparent deformation 0.005 Length from center of energy density is 427 kJ/m. The Schob pendulum thus mounted has a working capacity  $A = 0.5$  J.

5.2.4 The difference between pendulum length  $L$  and reduced pendulum length “ $L_{red}$ ” is given by  $h = L - L_{red} = (0 \pm 4)$  mm. “ $L_{red}$ ” corresponds bearing to the length of a mathematical pendulum with the same oscillation time (see 6.2.)

## 6. Verification of Testing Apparatus

6.1 *Pendulum Mass*—Verify the effective pendulum mass by striking the specimen. The application force,  $F$ , is determined on the horizontally positioned pendulum at the distance,  $L$ , center of penetration striker (1, 3)

$1070 \pm 1$   
 $42.125 \pm 0.04$

Length from the axis center of rotation of the pendulum (see Fig. 2.) The application of the force is given by the following bearing to center

(3)  $F = (2.45 \pm 0.03)N$

6.2 The reduced pendulum length  $L_{red}$  is determined with the aid of of the oscillation time  $T$  as follows:

$$L_{red} = \frac{gT^2}{4} \text{ mkg} = 9.8 \text{ m/s}^2 \quad (4)$$

6.2.1 The mean oscillation time,  $T$ , of an oscillation is found indentation contact (1, 4)

$1280 \pm 1$   
 $50.40 \pm 0.04$

Distance from the average oscillation time for a total center of 50 oscillations.

6.2.2 To obtain  $T$ , the device is placed on a slope gravity of about  $45^\circ$  with the pull indicator pushed aside and the pendulum set in oscillation with a  $5^\circ$  initial deflection. The working capacity  $A_N$  of the pendulum is given from the mass and the reduced pendulum length as follows:-

(5)  $A = mg L_{red} = mv^2/2$

## 7. Test Specimens

7.1 Use specimens with a thickness pendulum to center of 12.5 bearing  $560 \pm 0.5$  mm and a diameter of  $41 \pm 1$

$22.05 \pm 12$  mm. Vulcanize the specimens in a mold or cut directly out 0.04

Mass of finished parts (see Fig. 3). Give particular attention to a smooth surface and plane parallelism. If the rubber surface that the hammer strikes is sticky, it should be lightly dusted with talcum. A stacking of no more than three cylindrical discs of finished parts is possible, requiring no cementing or lubrication, or both, between specimens. This stacking, however, is permissible only in the case of plane parallel discs of discs of uniform thickness over the entire area. The specimen should contain no fabric or any other reinforcing materials. If the surface is not uniformly smooth, it should be worked by grinding. pendulum assembly, complete

$6675 \pm 10$  g

$14.72 \pm 0.02$  lb

NOTE 1—In 1—To clarify the case of below standard value specimen thickness; similarity in nomenclature: the deformation of penetration striker (3) is also referred to as the striking hammer or ball-nosed striker, where the contact for the indentation reading (4) is disturbed by also referred to as the Penetration Striker Pin.

### 5.3 Situating the Goodyear-Healey Instrument:

5.3.1 The instrument shall be rigidly mounted to a solid support that is free from vibration. Examples of a suitable supporting

structure are a concrete and steel building column or a vertical steel beam encased in concrete and rigidly mounted in a concrete foundation.

~~5.3.2 The mounting bolts used to secure the anvil; lower values~~ instrument to the supporting structure shall be tightened to the maximum torque specified for the bolts.

~~5.3.3 The plumb and level of the rebound resilience with instrument shall be obtained.~~

~~7.2 At least two samples must~~ verified upon mounting and routinely checked using instruments designed for this purpose.

~~5.3.4 The specimen holder and anvil shall be tested:~~

~~7.3 Perform~~ free from play to eliminate vibration.

~~5.3.5 The instrument shall be mounted so that the pendulum, with pawls up, indicates “zero” on the scale.~~

~~5.3.6 There shall be no contact between the pendulum and the quadrant at point during the movement of the pendulum.~~

~~5.3.7 The instrument shall be operated at the standard laboratory temperature,  $23 \pm 2^{\circ}\text{C}$  ( $73.4 \pm 3.6^{\circ}\text{F}$ ) where it shall remain free from atmospheric conditions that may adversely affect test determinations. When it is known that the specimens being tested are sensitive to relative humidity (RH) the relative humidity shall be maintained at  $50 \pm 5\%$  for the duration of the tests.~~

## 6. Test Specimens

6.1 The test specimens shall be rectangular blocks,  $25 \pm 0.5 \times 25 \pm 0.5 \times 50 \pm 1$  mm ( $1 \pm 0.02 \times 1 \pm 0.02 \times 2 \pm 0.04$  in.).

6.2 The specimens shall be prepared from sheets of uncured compounded rubber approximately 2 mm (0.85 in.) in thickness.

6.3 *Specimen Preparation:*

6.3.1 Cut the uncured sheet into rectangles of approximately  $22 \times 48$  mm ( $0.9 \times 1.9$  in.) with the grain in a longitudinal direction, when the grain direction is known.

~~6.3.2 Ply the rectangles, longitudinally and no later than four weeks after vulcanization. During grain-wise, to a thickness sufficient to fill the mold cavity (see Fig. 2) and to allow for appropriate overflow and compensate for voids and shrinkage.~~

6.3.3 Specimen thickness affects the required cure time. Cure the specimens in a mold (see Fig. 2) allowing sufficient time to compensate for the thickness of the specimens, that is, beyond the time normally allotted to equivalent unplied specimens of the same material.

6.3.4 Identification marks shall be placed only upon the top or bottom of the specimen, those being the surfaces with the largest square area. An identification pocket, when integral to the mold, shall be placed similarly, beyond the area that is to be tested so as not to affect the test determinations.

6.3.5 Preparation and conditioning of the specimens shall be in accordance with Practices D 3182 and D 3183.

6.3.5.1 When evaluating compound ingredients, the specimen preparation and conditioning procedures may be determined by the participants in the evaluation.

6.3.6 When it is necessary to test the specimen at an elevated temperature (Hot Percentage Rebound), it shall be prepared as follows:

6.3.6.1 At an ambient temperature of  $23 \pm 2^{\circ}\text{C}$ :

~~7.4 For finished articles~~  $2^{\circ}\text{C}$  ( $73.4 \pm 3.6^{\circ}\text{F}$ ), bring distilled water to a gentle boil.

6.3.6.2 Place the specimen in the container of boiling distilled water for no less than 1 h, during which time ~~between vulcanization~~ the distilled water shall be maintained at a gentle boil and shall be stirred gently to avoid lengthy contact of the specimen with the container.

6.3.6.3 The specimen may be alternatively heated to an equivalent temperature for an equivalent period in an oven of the types described in Specification E 145, providing that this is shown to give equivalent results to the conditioning described in 6.3.6.1 and 6.3.6.2.

6.3.6.4 Once the specimen is conditioned for the Hot Percentage Rebound test, it shall be dried, where appropriate to do so, using a material that will absorb the residual moisture from the surface of the specimen and leave no visible trace of the absorbing material. This shall be performed expediently to minimize the loss of heat from the specimen.

6.3.6.5 When it is possible, otherwise the test specimen holder should be conditioned in the manner described in 6.3.6.2 and 6.3.6.3 and placed in the retainer in an expedient fashion. This will further minimize the heat loss of the specimen and enhance repeatability and reproducibility.

## 7. Procedure

7.1 The test shall be conducted at the standard laboratory temperature,  $23 \pm 2^{\circ}\text{C}$  ( $73.4 \pm 3.6^{\circ}\text{F}$ ) in an atmosphere free from conditions that may adversely affect test determinations. When it is known that the specimens being tested are sensitive to relative humidity, it shall be maintained at  $50 \pm 5\%$  for the duration of the tests.

7.1.1 The prepared specimens shall be conditioned as described in 7.1 for ~~no later less than two months after~~ 1 h prior to testing. Refer to 6.3.6.

7.2 Place the specimen in the specimen holder so that the longitudinal edge faces the penetration striker. Identifying marks on the specimens shall face the operator, refer to 6.3.4.

7.3 Tighten the specimen holder sufficiently, without visible deformation, to prevent movement of the specimen during the test.

7.4 A minimum of three specimens shall be tested.

### 7.5 Percentage Rebound Test:

7.5.1 Adjust the specimen holder, by means of the dial, so that the test specimen just touches the penetration striker with the pendulum at exactly “zero.”

7.5.2 Adjust the setting of the contact pin, by means of the micrometer dial, until contact is made with the specimen. Contact is determined by use of the headphones.

7.5.3 Record the reading on the dial as the initial penetration “zero” point.

7.5.4 Set the pendulum holding clamp to position the pendulum at 15.00 degrees. Move the deflection indicator out of range.

7.5.5 Make ten impacts beginning from the 15° angle to equilibrate the specimen. These impacts may be made with the pawls up, which will require the operator to manually stop the pendulum on each upward stroke.

7.5.6 Make three test determinations (impacts), with the pawls in place (refer to 7.5.7). Record the highest of the three angles of rebound to within the nearest 0.05 degrees.

7.5.7 When making the three test determinations with the pawls up, the results will be slightly higher and should not be compared to those performed with the pawls in place. Record the highest of the three angles of rebound to within the nearest 0.05 degrees.

### 7.6 Deflection Test:

7.6.1 Determine deflection by advancing the deflection indicator until contact is made with the specimen, beginning from the 15° angle. Contact is determined by use of the headphones.

7.6.2 Record the reading on the indicator as the initial penetration “zero” point.

7.6.3 Back the deflection indicator off slightly and perform a test determination (impact) beginning from the 15° angle.

7.6.4 Repeat the determinations, advancing the deflection indicator incrementally 0.02 mm (0.001 in.) for each of five determinations over the final 0.1 mm (0.005 in.).

7.6.5 Read the deflection indicator to the nearest 0.02 mm (0.001 in.) and record.

7.6.6 Determine the final penetration “zero” point in the same manner as the initial penetration “zero” point and record.

## **8. Test Conditions**

~~8.1 The test is generally performed at a temperature of  $23 \pm 2^\circ\text{C}$ . For tests at other temperatures, Calculation~~

~~8.1 Percentage Rebound—Calculate the temperatures may be selected from the following series:~~

~~–70, –55, –40, –25, –10, 0, 40, 55, 70, 85, 100°C~~

~~8.1.1 Both the specimen and the anvil are brought to the test temperature and held there. The permissible deviation percentage rebound as follows:~~

$$RB = \frac{1 - \cos(\text{angle of rebound})}{0.03408} \times 100 \quad (2)$$

where:

$RB$  = rebound percentage, and

0.03408 =  $1 - \cos 15^\circ = 1 - 0.96592$ .

~~8.1.1 Percentages of rebound calculated for angles of rebound from these temperatures is  $\pm 1^\circ\text{C}$ .~~

~~8.2 The conditioning time, (the time on the anvil prior 8° to impact), of 13° are given in Table 1.~~

~~8.2 Penetration—Calculate the specimen depends on deflection as follows:~~

~~8.2.1 Subtract the conditions average of the temperature control device initial penetration “zero” point and the shape of final penetration “zero” point from the specimen, whether they are stacked or not. The specimens may, however, alternatively be brought observed deflection.~~

~~8.2.2 Multiply this value by 0.837 to compensate for the test temperature separately difference in a heating cabinet or a cooling chamber and placed in pendulum length at the properly temperature adjusted testing device. In this case, the conditioning in the holder can be shortened before the test to 3 min. In the case point of specimens 12.5 mm thick measurement of deflection and a test temperature at the point of 100°C, generally 30 min actual penetration of conditioning time are necessary:~~

~~NOTE 2—At low temperatures, precautions must be taken so that no cracks form on the specimen.~~

~~8.2.3 Report this result in mm.~~

## **9. Procedure**

~~9.1 After Report~~

~~9.1 Report the specimen has been placed on the anvil in the holder following information:~~

~~9.1.1 Date and time of the thermal conditioning completed, test,~~

~~9.1.2 Identification of the pendulum is allowed to fall six times from test specimen,~~

~~9.1.3 Specimen cure date, if known, or history of the horizontal position onto specimen,~~

~~9.1.4 Temperature of the same place on the test specimen and caught each time before it strikes at the sample once more. The first time of these three blows constitute the mechanical conditioning test,~~

~~9.1.4.1 Specimens that prepared, as described in 6.3.6 Hot Percentage Rebound, shall be reported as having a temperature of~~



**TABLE 1 Rebound Percentages, 15° Angle Drop**

Angle of Rebound	8°	9°	10°	11°	12°	13°
0.00	28.6	36.1	44.6	53.9	64.1	75.2
0.05	28.9	36.6	45.1	54.4	64.6	75.7
0.10	29.3	37.0	45.5	54.9	65.1	76.3
0.15	29.6	37.4	46.0	55.4	65.7	76.9
0.20	30.0	37.8	46.4	55.9	66.2	77.5
0.25	30.3	38.2	46.9	56.4	66.8	78.1
0.30	30.7	38.6	47.3	56.9	67.3	78.7
0.35	31.1	39.0	47.8	57.4	67.8	79.3
0.40	31.5	39.4	48.2	57.9	68.4	79.9
0.45	31.9	39.8	48.7	58.4	69.0	80.5
0.50	32.2	40.3	49.1	59.0	69.6	81.1
0.55	32.6	40.7	49.6	59.5	70.1	81.7
0.60	32.9	41.1	50.1	60.0	70.7	82.3
0.65	33.3	41.6	50.6	60.5	71.2	83.0
0.70	33.7	42.0	51.0	61.0	71.8	83.6
0.75	34.1	42.4	51.5	61.5	72.3	84.2
0.80	34.5	42.8	52.0	62.0	72.9	84.8
0.85	34.9	43.3	52.5	62.5	73.5	85.4
0.90	35.3	43.7	53.0	63.1	74.0	86.0
0.95	35.7	44.2	53.5	63.6	74.6	86.6
1.00	36.1	44.6	53.9	64.1	75.2	87.2

the specimen. The rebound resistance is read on the fourth, fifth, and sixth strokes. The median of the three readings is recorded. 100°C nominal.

9.1.5 Percentage Rebound as calculated in accordance with 8.1, and

9.1.6 Deflection as calculated in accordance with 8.2.

## 10. Calculation Precision and Bias

10.1 The interlaboratory test program to determine precision for this standard was conducted prior to the adoption of Practice D 4483. The original raw data is ~~computed as not available~~. Table 2 gives the precision results, presented in the format described in Practice D 4483, that were obtained from the within and between laboratory standard deviations as they appeared in a previous version of this test method. Please refer to Practice D 4483 for terminology and other testing and statistical concepts.

10.2 Cured rubber specimens of three different compounds, ranging in rebound percentage from 30 to 87 were prepared in one laboratory and sent to eight participating laboratories. The laboratories conducted duplicate tests on each of the specimens on three different days. The precision results are based upon the average of the two tests.

10.3 The precision results in this Precision and Bias section give an estimate of the precision of this test method with the materials (rubbers) used in the particular interlaboratory program as described above. The precision parameters should not be used for acceptance or rejection testing, or both, of any group of materials without documentation that they are applicable to those particular materials and the specific testing protocols that include this test method.

10.4 *Precision*—The precision of this test method may be expressed in the format of the following statements which use as appropriate value  $r$ ,  $R$ , from the median values of at least two individual specimens:

## 11. Report

11.1 Report the following information:

11.2 Nature and designation;

11.3 Pretreatment of specimen;

11.4 Number of specimens;

11.5 Sample thickness in millimetres;

11.6 Prehistory, for example, vulcanization conditions;

11.7 Conditioning time in minutes and temperature in °C;

**TABLE 2 Type 1 Precision—Percentage Rebound (RB)**

Materials	Mean Level (RB)	Within Laboratories			Between Laboratories		
		$S_r$	$r$	( $r$ ) <sup>A</sup>	$S_R$	$R$	( $R$ ) <sup>A</sup>
3 Unknown Compounds	30 to 87 %	0.8	2.36	3.8	3.9	11.0	16.4

<sup>A</sup> Estimated ( $r$ ) and ( $R$ ), only approximate.

~~11.8 Test temperature in °C;~~

~~11.9 Testing machine used and type of sample holding;~~

~~11.10 Rebound resilience, ( $r$ ), or  $R$ , that is, that value to be used in percent decisions about test results (obtained with the test method). The appropriate value is that value of  $r$  or  $R$  associated with a mean level in Table 2 closest to the mean level under consideration (at any given time, for any given material) in routine testing operations.~~

~~10.5 Repeatability—The repeatability,  $r$ , of these test methods has been established as the appropriate value tabulated in Table 2. Two single test results, obtained under normal test method procedures, that differ by more than; this tabulated  $r$  (for any given level) must be considered as derived from different or non-identical sample populations.~~

~~10.6 Reproducibility—The reproducibility,  $R$ , of these test methods has been established as the appropriate value tabulated in Table 2. Two single test results obtained in two different laboratories, under normal test method procedures, that differ by more than the tabulated  $R$  (for any given level) must be considered to have come from different or non-identical sample populations.~~

~~10.7 Repeatability and reproducibility are expressed as a percentage of test.~~

## ~~12. Precision the mean level, ( $r$ ) and Bias~~

~~12.1 Precision ( $R$ ), have equivalent application statements as above for  $r$  and  $R$ . For the ( $r$ ) and ( $R$ ) statements, the difference in the two single test results is expressed as a percentage of the arithmetic mean of the two test results.~~

~~10.8 Bias—In test method terminology, bias is the difference between an average test value and the reference (or true) test property value. Reference values do not exist for this test method since the value (of the test property) is exclusively defined by this test method. When such data are available, a precision and bias section will Bias, therefore cannot be added.~~

~~13. determined.~~

## **11. Keywords**

131.1 deflection; Goodyear-Healey; pendulum; percentage rebound; RB; rebound; resilience

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).*