



Designation: F 1877 – 98 (Reapproved 2003)^{ε1}

Standard Practice for Characterization of Particles¹

This standard is issued under the fixed designation F 1877; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

^{ε1} NOTE—Editorial changes were made throughout in April 2003.

1. Scope

1.1 This practice outlines a series of procedures for characterization of the morphology, number, size, and size distribution of particles. The methods utilized include sieves, optical, SEM, and electrooptical.

1.2 These methods are appropriate for particles produced by a number of different methods. These include wear test machines, total joint simulation systems, abrasion testing, methods for producing particulates, such as shatter boxes or pulverizers, commercially available particles, and particles harvested from tissues in animal or clinical studies.

1.3 The debris may include metallic, polymeric, ceramic, or any combination of these.

1.4 The digestion procedures to be used and issues of sterilization of retrieved particles are not the subject of this practice.

1.5 A classification scheme for description of particle morphology ~~are~~ is included in Appendix X3.

1.6 As a precautionary measure, removed debris from implant tissues should be sterilized or minimally disinfected by an appropriate means that does not adversely affect the particulate material. *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*

E 11—Specification

¹ This practice is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.16 on Biocompatibility Test Methods.

Current edition approved April 10, 1998; 2003. Published May 2003. Originally approved in 1998. Last previous edition approved in 1998 as F 1877 – 98.

~~C 678 Test Methods for Wire-Cloth Sieves for Testing Purposes~~ Particle Size Distribution of Alumina or Quartz by Electric Sensing Technique²

~~E 20 Practice 11 Specification for Particle Size Analysis of Particulate Substances in the Range of 0.2 to 75 μm by Optical Microscopy~~ Wire Cloth and Sieves for Testing Purposes³

E 161 Specification for Precision Electroformed Sieves (Square Opening Series)^{2,3}

E 1617 Practice for Reporting Particle Size Characterization Data³

E 766 Practice for Calibrating the Magnification of Scanning Electron Microscopes (SEMs)⁴

F 561 Practice for Retrieval and Analysis of Implanted Medical Devices, and Associated Tissues⁵

F 660 Practice for Comparing Particle Size in the Use of Alternative Types of Particle Counters⁶

F 661 Practice for Particle Count and Size Distribution Measurement in Batch Samples for Filter Evaluation Using an Optical Particle Counter⁷

F 662 Method for Particle Count and Size Distribution in Batch Samples for Filter Evaluation Using an Electrical Resistance Particle Counter⁷

~~F 690 Particle Size Distribution~~ 732 Test Method for Wear Testing of Alumina or Quartz by Electric Sensing Technique²
Polymeric Materials for Use in Total Joint Prostheses⁵

~~F 732 Practice 1714 Guide for Reciprocating Pin-on-Flat Evaluation of Friction and Gravimetric Wear Properties Assessment of Polymeric Materials for Use~~ Prosthetic Hip Designs in Total Joint Prostheses⁴ Simulator Devices⁵

~~F 1714~~ 5 Guide for Gravimetric Wear Assessment of Prosthetic Hip Designs in Simulator Devices⁴

~~F 1715~~ Guide for Gravimetric Wear Assessment of Prosthetic Knee Designs in Simulator Devices⁵

3. Terminology

3.1 *Definitions of Terms Specific to This Standard:*

3.1.1 *agglomerate, n*—a mass formed by the cementation of individual particles, probably by chemical forces.

3.1.2 *aggregate, n*—a mass formed of mixtures of particulate and agglomerate particles having a binding force intermediate between agglomerates and flocculates. Formation of aggregates can occur after sampling if the samples are improperly kept or treated.

3.1.3 *aspect ratio (AR), n*—a ratio of the major to the minor diameter of a particle, which can be used when the major axis does not cross a particle outline (see 11.3.3).

3.1.4 *elongation (E), n*—ratio of the particle length to the average particle width (see 11.3.4).

3.1.5 *equivalent circle diameter (ECD), n*—a measure of the size of a particle (see 11.3.2 and Appendix X1).

3.1.6 *Feret diameter, n*—the mean value of the distance between pairs of parallel tangents to a projected outline of a particle.

3.1.7 *flocculate, n*—a group of two or more attached particles held together by physical forces, such as surface tension, adsorption, or similar forces.

3.1.8 *form factor (FF), n*—a dimensionless number relating area and perimeter of a particle, as ~~directed~~ determined in 11.3.6.

3.1.9 *irregular, adj*—a particle that cannot be described as round or spherical. A set of standard nomenclature and reference figures are given in Appendix X2.

3.1.10 *particle, n*—the smallest discrete unit detectable as determined in ~~F test M~~ methods.

3.1.11 *particle breadth, n*—distance between touch points of the shortest Feret pair, orthogonal to length.

3.1.12 *particle length, n*—distance between touch points of maximum Feret pair. This value will be greater than or equal to the maximum Feret diameter.

3.1.13 *rectangular, adj*—a particle that approximates a square or rectangle in shape.

3.1.14 *roundness (R), n*—a measure of how closely an object represents a circle as determined in 11.3.5.

3.1.15 *spherical, adj*—a particle with a generally spherical shape that appears round in a photograph.

4. Summary of Practice

4.1 Particles produced by implant wear *in vivo* in animal or clinical studies are harvested from tissues after digestion utilizing methods, such as those in Practice F 561. Particles generated *in vitro*, or obtained from commercial sources, are used as received, or after digestion, if they were generated in protein solutions, and further separation if there are signs of aggregation. A two level analysis is provided. For routine analysis, the particles are characterized by the terms of morphology and by size using Feret diameters. For more detailed studies, several methods are described that may be utilized for numerically characterizing their dimensions, size distribution, and number.

² Discontinued; See 1995 *Annual Book of ASTM Standards*, Vol 14.02.

³ ~~Discontinued 1994~~—Vol *Annual Book of ASTM Standards*, Vol 14.02.

⁴ *Annual Book of ASTM Standards*, Vol 14.03.01.

⁵ The examples provided were analyzed with the NIH Image Program by Landry and Agarwal. A set

⁵ *Annual Book of macros is available from the Department of Orthopaedics, University of Texas Health Science Center at San Antonio. ASTM Standards*, Vol 13.01.

⁶ Lator, P., donated photographs from Howmedica R and D laboratories.

⁶ *Annual Book of ASTM Standards*, Vol 11.01.

⁷ Szivek J.A., donated sample set.

⁷ Discontinued; See 2001 *Annual Book of ASTM Standards*, Vol 14.04.

5. Significance and Use

5.1 The biological response to materials in the form of small particles, as from wear debris, often is ~~different~~ significantly different from that to the same materials as larger implant components. The size and shape (morphology) of the particles may have a major effect on the biological response; therefore, this practice provides a standardized nomenclature for describing particles. Such a unified nomenclature will be of value in interpretation of biological tests of responses to particles, in that it will facilitate separation of biological responses associated with shape from those associated with the chemical composition of debris.

5.2 The quantity, size, and morphology of particles released as wear debris from implants *in vivo* may produce an adverse biological response which will affect the long term survival of the device. Characterization of such debris will provide valuable information regarding the effectiveness of device designs or methods of processing components and the mechanisms of wear.

5.3 The morphology of particles produced in laboratory tests of wear and abrasion often is affected by the test conditions, such as the magnitude and rate of load application, device configuration, and test environment. Comparison of the morphology and size of particles produced *in vitro* with those produced *in vivo* will provide valuable information regarding the degree to which the method simulates the *in vivo* condition being modeled.

6. Interferences

6.1 Particles may form aggregates or agglomerates during preparation and storage. These would result in an increase in measured particle size and decrease in particle number. It is essential that care be taken to resuspend particles prior to analysis and to note any effects of the dispersant used.

6.2 Debris from wear tests or harvested from tissues may contain a mixture of materials. Care should be taken to separate the particles and methods utilized to determine the chemical composition of the particles.

6.3 Many automated particle counters operate on the assumption that the particles are spherical. These methods may not be appropriate for nonspherical debris. Additional methods should be used to verify size using methods that take aspect ratio into consideration, for example, SEM image analysis.

7. Apparatus

7.1 Scanning Electron Microscope (SEM):

7.1.1 Standard SEM equipment can be utilized for many studies. In special instances, such as with polymeric particles, a low acceleration voltage (1-2 kV) machine with a high brightness electron source, such as a field emission tip, may be utilized.

7.1.2 Elemental analysis may be accomplished with an energy dispersive spectrometer (EDS) for energy dispersive X-ray analysis (EDXA).

7.2 *Optical Microscope*—An optical microscope operating in the transmission mode may be utilized. Dark field illumination may enhance visualization of some particles. Polarized light will facilitate identification of semicrystalline polymeric materials.

7.3 Automatic Particle Counters (see Practice F 660):

7.3.1 *Image Analyzer*— This instrument counts particles by size as those particles lie on a microscope slide.

7.3.2 *Optical Counter*— This instrument measures the area of a shadow cast by a particle as it passes a window. From this area the instrument reports the diameter of a circle of equal area (see Practice F 661).

7.3.3 *Electrical Resistance Counter* —This instrument measures the volume of an individual particle. From that volume the instrument reports the diameter of a sphere of equal volume (see Method F 662).

8. Reagents

8.1 *Particle-Free (0.2 μm Filtered) Deionized Water*, for nonpolymeric particles.

8.2 *Particle-Free (0.2 μm Filtered) Methanol or Ethanol*, for polymeric or mixed debris.

8.3 *Ultra-Cleaning Reagent*, for apparatus or labware cleaning.

9. Specimen Preparation

9.1 Specimens from explanted tissues from animal or clinical studies may need to be harvested and digested using methods, such as those described in Practice F 561.

9.2 Particles from *in vitro* cell culture tests also may need to be digested and harvested.

9.3 PCentrifugation of particles from wear tests should may be centrifuged considered, if necessary, at atleast 400 g for 10 min, and resuspended in water or methanol. Resuspended particles may be filtered in accordance with Practice F 561 prior to examination by SEM.

10. Particle Imaging by Light or Scanning Electron Microscopy

10.1 Images may either be captured electronically or photographically for subsequent analysis.

10.2 For the characterization and measurements to be accurate, it is essential that the particles be imaged at the largest magnification as possible. The magnifications in Table 1 are recommended.

10.3 For particle size distribution measurements, divide each of the size ranges specified in Table 1, into 10 bins.

TABLE 1 Recommended Magnifications for Particle Imaging

Magnification	Particle Size Range (µm)
10000	0.1 to 1.0
1000	1 to 10
100	10 to 100

11. Particle Characterization

11.1 *Particle Shape (Morphology)* —Refer to the photographs and classify the morphology of the particles using the nomenclature in Appendix X2.

11.2 *Routine Particle Size Determination Using Feret Diameters:*

11.2.1 The use of multiple Feret diameters especially is useful for spherical and rectangular particles.

11.2.2 Determine the particle size and aspect ratio as the mean of two Feret diameters.

11.2.3 Calculate the particle size distribution based on the volume of solution used and the size of the filters.

11.3 *Detailed Particle Shape Analysis for Irregular Shaped Particles:*

11.3.1 Five particle dimensional measurements are provided using examples shown in Appendix X1.⁸ One is a measure of particle size while the other four are shape descriptors.

11.3.2 *The Equivalent Circle Diameter (ECD) as a Measure of Particle Size:*

11.3.2.1 The ECD is defined as the diameter of a circle with an area equivalent to the area (A) of the particle and has the units of length:

$$ECD = (4A/\pi)^{1/2} \quad (1)$$

11.3.3 *The Aspect Ratio (AR) is a Common Measure of Shape:*

11.3.3.1 The AR is the ratio of the major diameter (d_{max}) to the minor diameter (d_{min}). The major diameter is the longest straight line that can be drawn between any two points on the outline. The minor diameter is the longest line perpendicular to the major diameter:

$$AR = d_{max}/d_{min} \quad (2)$$

11.3.4 The elongation (E), is similar to the AR except it is more suited for the measurement of much longer particles, especially fibrillar particles, where the major axis line does not stay within the particle boundaries. Refer to particle types A and C in Appendix X1.

11.3.4.1 The E is the ratio of the length (FL) to the breadth (FW):

$$E = FL/FW \quad (3)$$

11.3.5 The roundness (R) is a measure of how closely a particle resembles a circle. The R varies from zero to one in magnitude with a perfect circle having a value of one.

$$R = (4A)/(\pi d_{max}^2) \quad (4)$$

where:

A = area, and

d_{max} = the maximum diameter.

11.3.6 The form factor (FF) is similar to R but is based on the perimeter (p) of the particle outline rather than the major diameter. The FF is more sensitive to the variations in roughness of the particle outline.

$$FF = 4\pi A/p^2 \quad (5)$$

where:

p = perimeter of the particle outline.

11.4 *Other Particles Size Determination Methods:*

11.4.1 Particles larger than 20 µm may be determined by sieves described in Specifications E 11 and E 161.

11.4.2 Particles in liquid suspension may be sized as directed in Practice F 661 or Method F 662.

12. Elemental Analysis

12.1 SEM-EDS analysis should be conducted at a magnification suggested in 10.2.

12.2 Elemental analysis should be conducted for at least 10 s for each particle. Since detailed compositional analysis is of questionable meaning for micron and submicron sized particles, it is recommended that composition be determined based on identification of key elemental peaks for the major elements likely to be present in the sample.

⁸Jacobs J.J.;

⁸The examples provided were analyzed with the NIH Image Program by Landry and Urban R.M., donated photograph: Agarwal. A set of macros is available from the Department of Orthopaedics, University of Texas Health Science Center at San Antonio.

13. Report

13.1 Report the following information:

- 13.1.1 The source of the particles and materials and methods for generation.
- 13.1.2 Methods utilized to digest and separate the particles.
- 13.1.3 Morphological description of the particles.
- 13.1.4 Results of particle size and shape analysis.

14. Precision and Bias

14.1 The precision and bias of this practice has not been determined.

15. Keywords

15.1 biocompatibility; morphology; particles; SEM; wear debris

APPENDIXES

(Nonmandatory Information)

X1. SAMPLE FIGURES FOR CALCULATION OF PARTICLE SIZE AND SHAPE

X1.1 See Fig. X1.1.

X2. NOMENCLATURE FOR PARTICLE MORPHOLOGY DESCRIPTION

X2.1 This collection is not intended to be all inclusive, but rather to provide a frame work for describing the morphology of particles.

NOTE X2.1—These figures are used as illustrative examples. Sources are indicated in parentheses (used with permission).

X2.1.1 *Spherical or Spheroidal:*

X2.1.1.1 Smooth, round (Fig. X2.1).⁹

X2.1.1.2 Smooth, oblong (Fig. X2.1).⁹

X2.1.1.3 Agglomerated, red blood cell - like (Fig. X2.2).¹⁰

X2.1.1.4 Rough (Fig. X2.3).⁹

X2.1.1.5 Spongy, porous (Fig. X2.4).¹¹

X2.1.2 *Granular, Irregular:*

X2.1.2.1 Smooth (Fig. X2.5).¹²

X2.1.2.2 Rough (Fig. X2.6).¹³

X2.1.2.3 Porous (Fig. X2.7).¹³

X2.1.2.4 Angulated (Fig. X2.8).¹⁴

X2.1.2.5 Fines, too small to characterize accurately (Fig. X2.9).⁹

X2.1.3 *Globular:*

⁹ Margevicius K.J., Bauer T.W., McMahon J.T., Brown S.A., Merritt K., "Isolation

⁹ Lalor, P., donated photographs from Howmedica R and Characterization of Debris in Membranes Around Total Joint Prostheses," *J Bone Joint Surg*, 76A:1664-1675, 1994. D laboratories.

¹⁰ Kieswetter K., Bauer T.W., Brown S.A., Van Lente F., Merritt K., "Characterization of Calcium Phosphate Powders by ESCA and EDXA," *Biomaterials*, 15:183-188, 1994.

¹⁰ Szivek J.A., donated sample set.

¹¹ Lerouge S., Huk O., Yahia L.H., Sedel L., "Characterization of In Vivo Wear Debris from Ceramic-Ceramic Total Hip Arthroplasties," *J Biomed Mater Res*, 32:627-633, 1996.

¹¹ Jacobs J.J., and Urban R.M., donated photograph.

¹² Hailey J.L., Ingham E., Stone M., Wroblewski B.M., Fisher J., "Ultra-High Molecular Weight Polyethylene Wear Debris Generated In Vivo

¹² Margevicius K.J., Bauer T.W., McMahon J.T., Brown S.A., Merritt K., "Isolation and in-Laboratory Tests: the Influence Characterization of Counterface Roughness," Debris in Membranes Around Total Joint Prostheses," *Proc Inst Mech Eng J Bone Joint Surg*, 210:3-10, 1996; 76A:1664-1675, 1994.

¹³ Campbell, P., donated photographs.

¹³ Kieswetter K., Bauer T.W., Brown S.A., Van Lente F., Merritt K., "Characterization of Calcium Phosphate Powders by ESCA and EDXA," *Biomaterials*, 15:183-188, 1994.

¹⁴ Shanbhag A.S., donated photograph.

¹⁴ Lerouge S., Huk O., Yahia L.H., Sedel L., "Characterization of In Vivo Wear Debris from Ceramic-Ceramic Total Hip Arthroplasties," *J Biomed Mater Res*, 32:627-633, 1996.

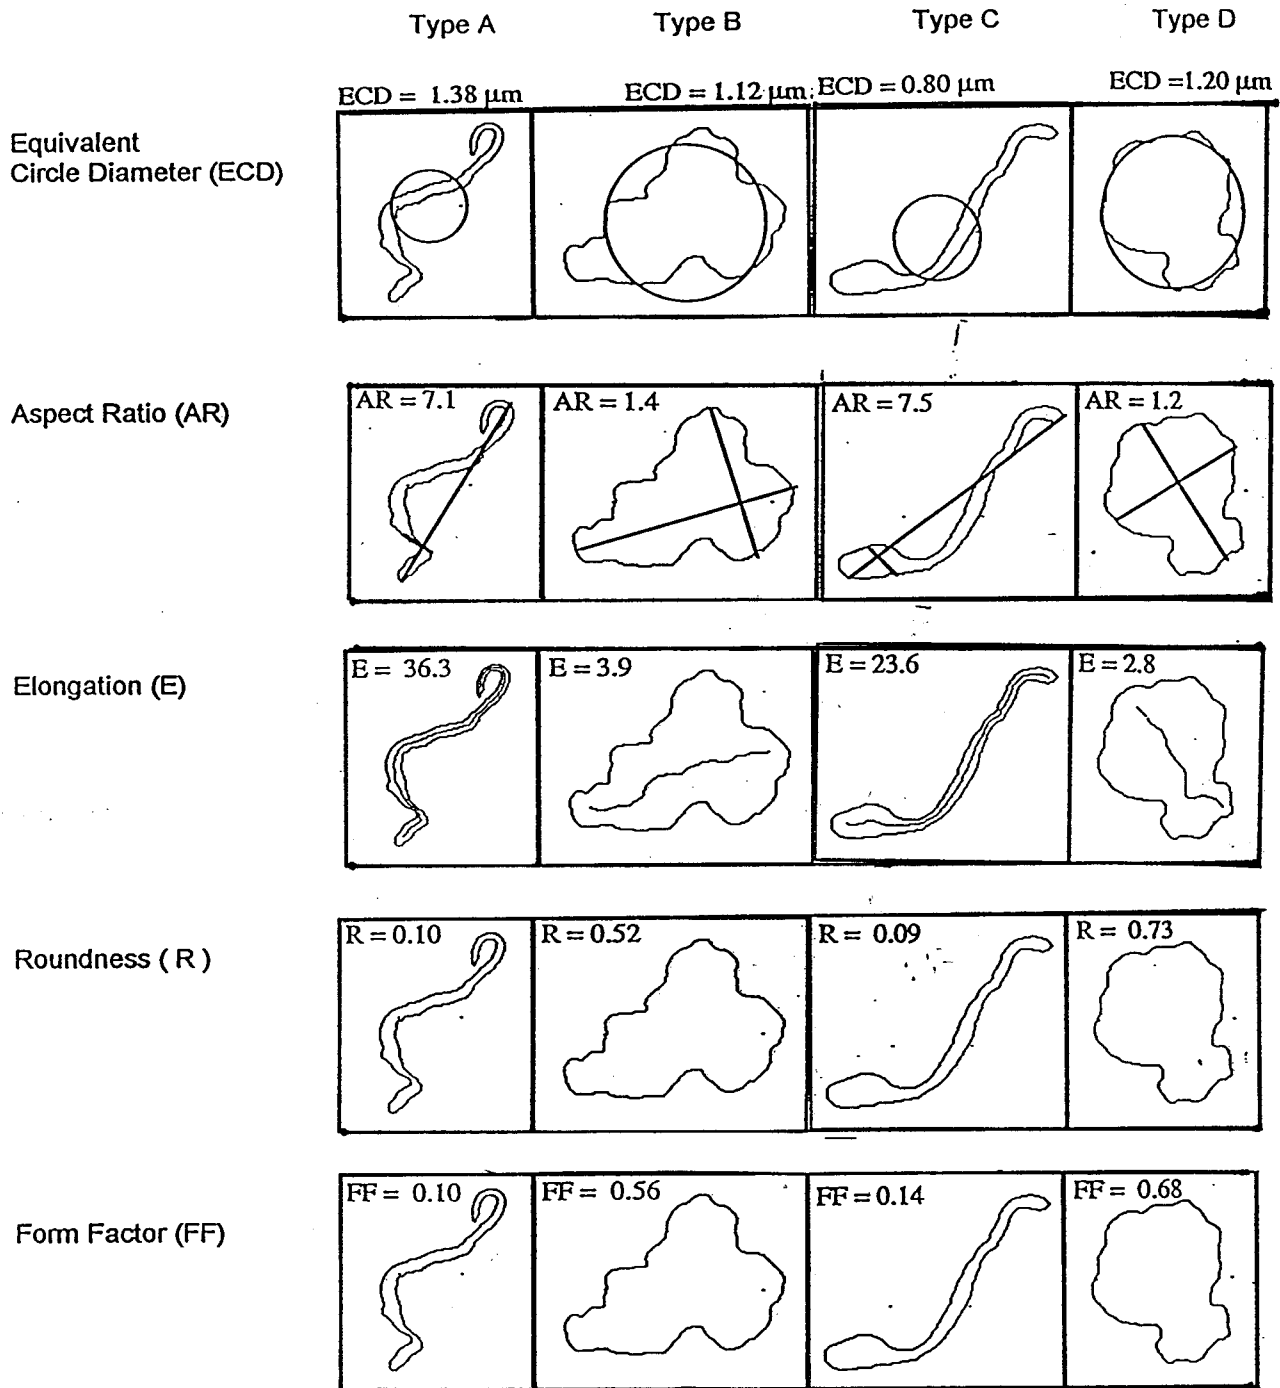


FIG. X1.1 Sample Figures for Calculation of Particle Size and Shape

X2.1.3.1 Clumped, florets, cauliflower (Fig. X2.10).¹⁵

X2.1.3.2 Agglomerated, diffuse (Fig. X2.11).¹⁶

X2.1.4 Flakes:

¹⁴ Bauer T.W., donated photograph.

¹⁵ Hailey J.L., Ingham E., Stone M., Wroblewski B.M., Fisher J., "Ultra-High Molecular Weight Polyethylene Wear Debris Generated *In Vivo* and in Laboratory Tests: the Influence of Counterface Roughness," *Proc Inst Mech Eng*, 210:3-10, 1996.

¹⁶ This practice is under the jurisdiction of ASTM Committee F04 on Medical and Surgical Materials and Devices and is the direct responsibility of Subcommittee F04.16 on Biocompatibility Test Methods.

Current edition approved Apr. 10, 2003. Published May 2003. Originally approved in 1998. Last previous edition approved in 1998 as F 1877 - 98.

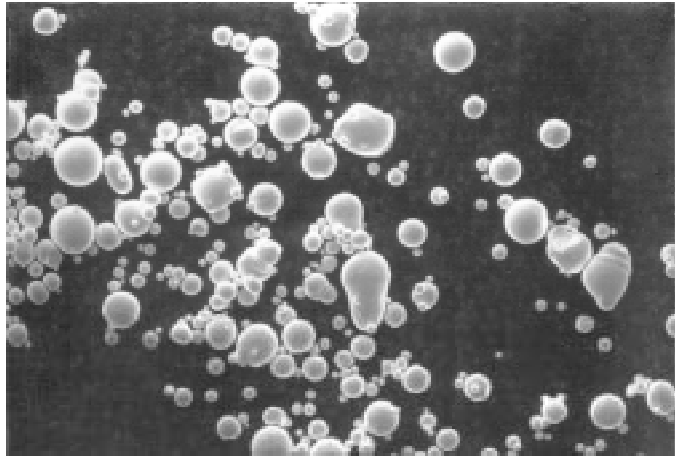


FIG. X2.1 Spherical or Spheroidal—Smooth, Round or Oblong

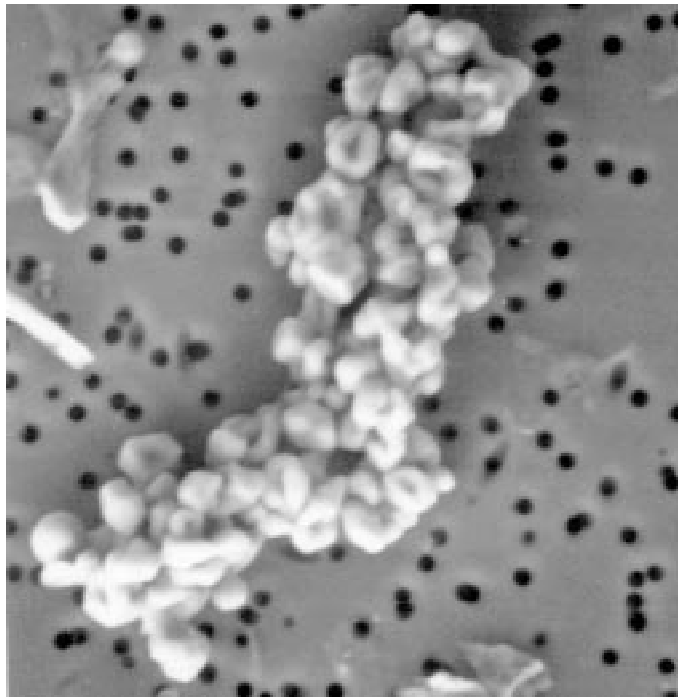


FIG. X2.2 Spherical or Spheroidal—Agglomerated Red Blood Cell-Like

- X2.1.4.1 Smooth (Fig. X2.12).¹⁵
- X2.1.4.2 Roughened (Fig. X2.13).¹⁵
- X2.1.4.3 Irregular (Fig. X2.14).¹⁶
- X2.1.4.4 Shards (probably thin cross sections of flakes) (Fig. X2.15).⁹
- X2.1.5 *Fibrillar*:
- X2.1.5.1 Straight (Fig. X2.16).¹⁰
- X2.1.5.2 Twisted (Fig. X2.17 and Fig. X2.18).¹⁰
- X2.1.5.3 Hammerhead (Fig. X2.19 and Fig. X2.18).¹⁶
- X2.1.5.4 Tadpole (Fig. X2.19).¹⁶
- X2.1.5.5 Seahorse (Fig. X2.18).¹⁶
- X2.1.6 *Sharps or Shards*:
- X2.1.6.1 Flakes, stacked sheets (Fig. X2.20).¹⁷

¹⁷ Shanbhag A.S., donated photograph.

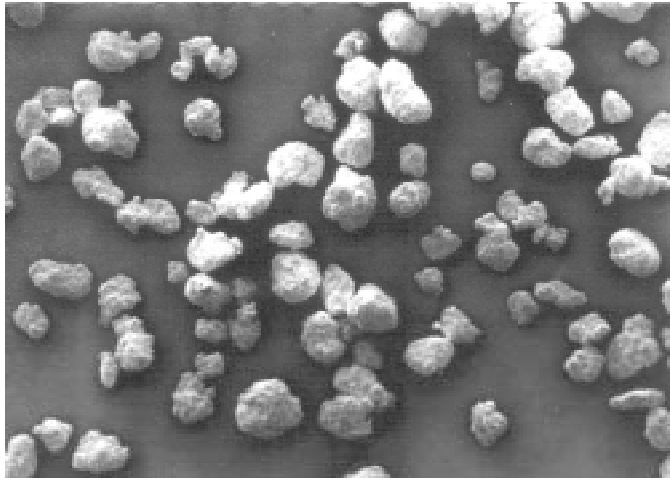


FIG. X2.3 Spherical or Spheroidal—Rough

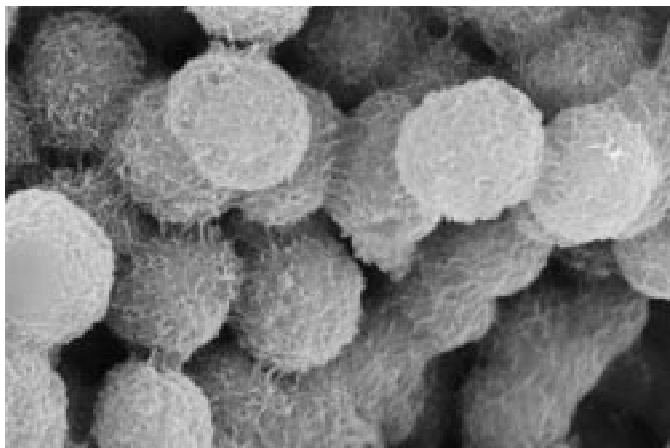


FIG. X2.4 Spherical or Spheroidal—Spongy, Porous

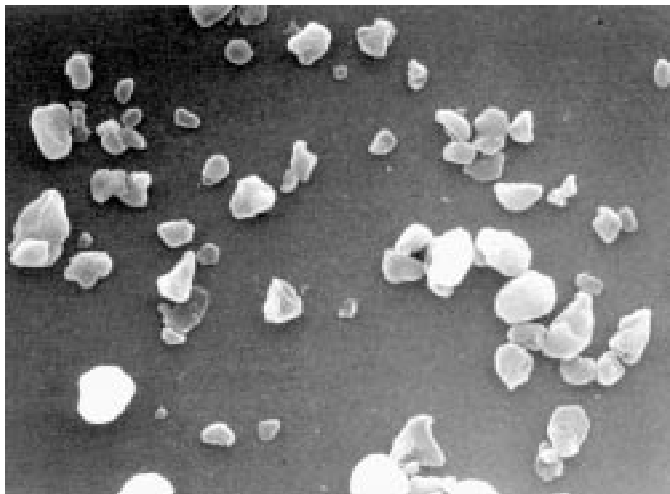


FIG. X2.5 Granular, Irregular—Smooth

X2.1.6.2 Rectangular, fibers (Fig. X2.21).¹⁸

X2.1.6.3 Lathe-like (Fig. X2.22).^{10,13}

¹⁸ Bauer T.W., donated photograph.



FIG. X2.6 Granular, Irregular—Rough

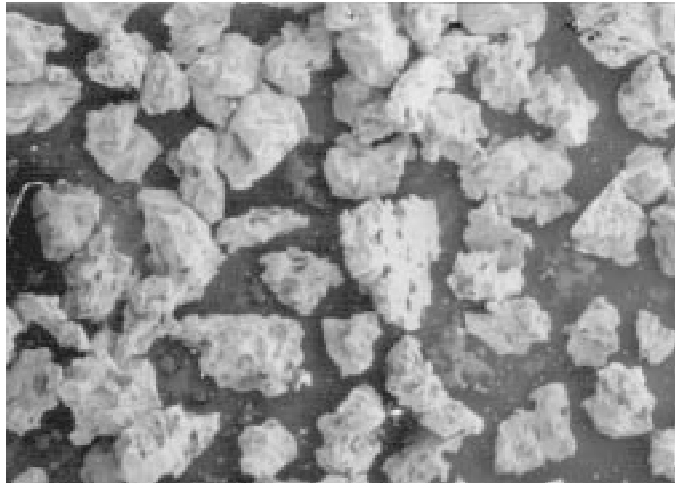


FIG. X2.7 Granular, Irregular—Porous

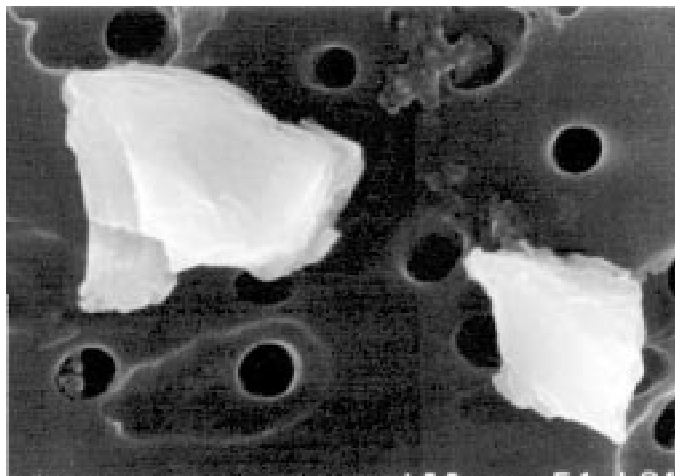


FIG. X2.8 Granular, Irregular—Angulated

X2.1.6.4 Cuttlefish (Fig. X2.23).¹⁵

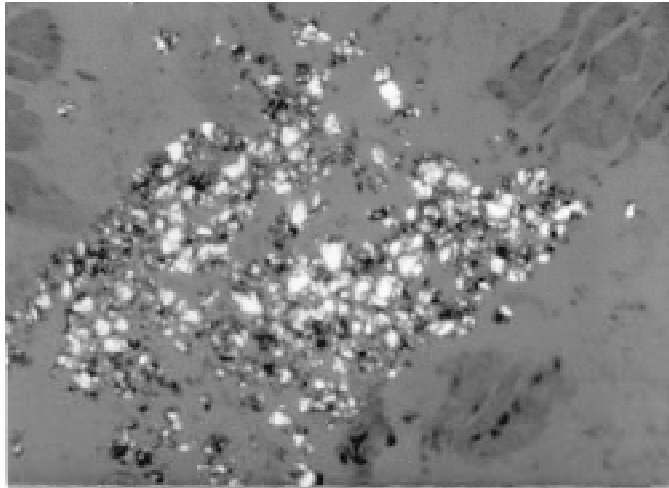


FIG. X2.9 Granular, Irregular—Fines Too Small to Characterize Accurately

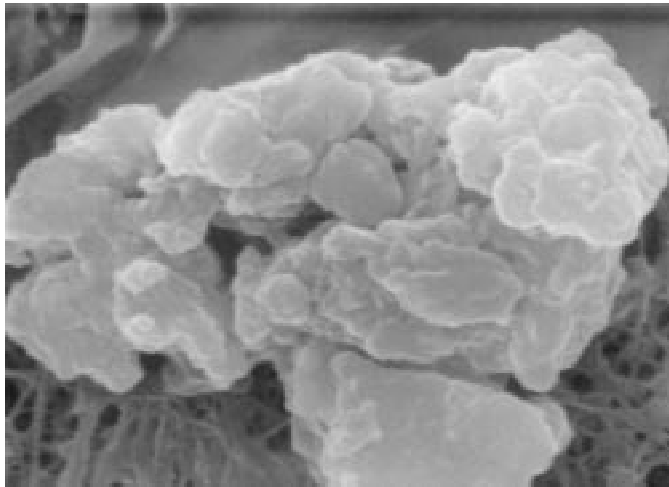


FIG. X2.10 Globular—Clumped, Florets, Cauliflower

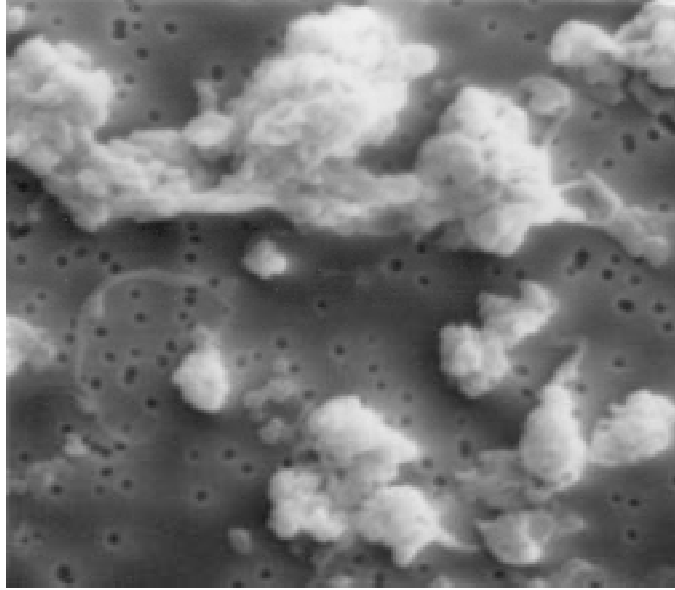


FIG. X2.11 Globular—Agglomerated, Diffuse

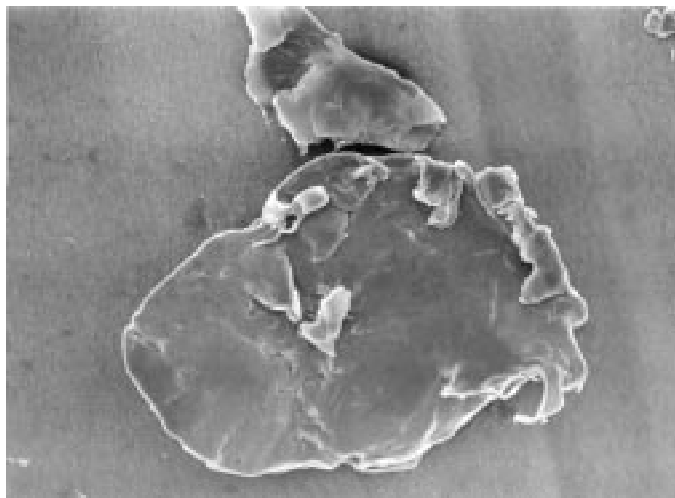


FIG. X2.12 Flakes—Smooth

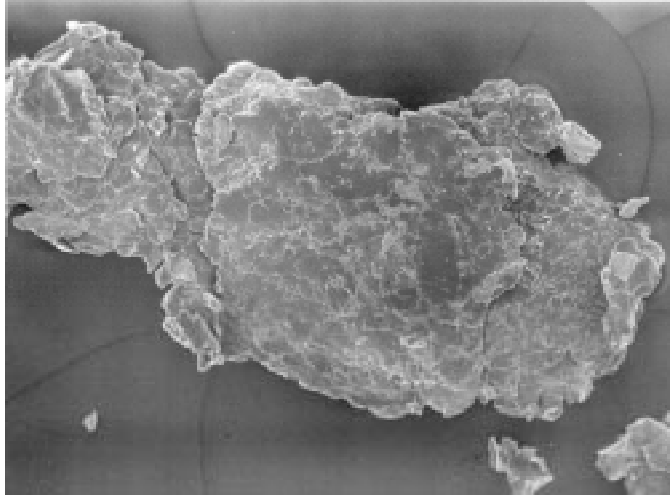


FIG. X2.13 Flakes—Roughened

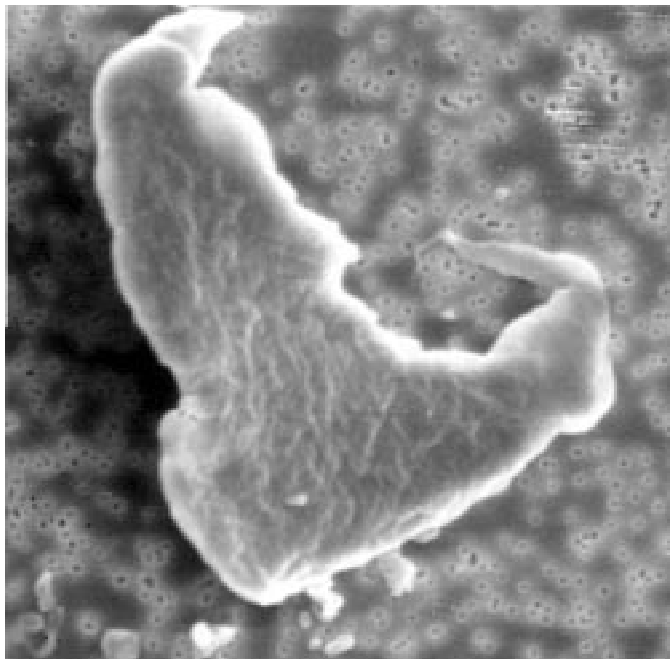


FIG. X2.14 Flakes—Irregular

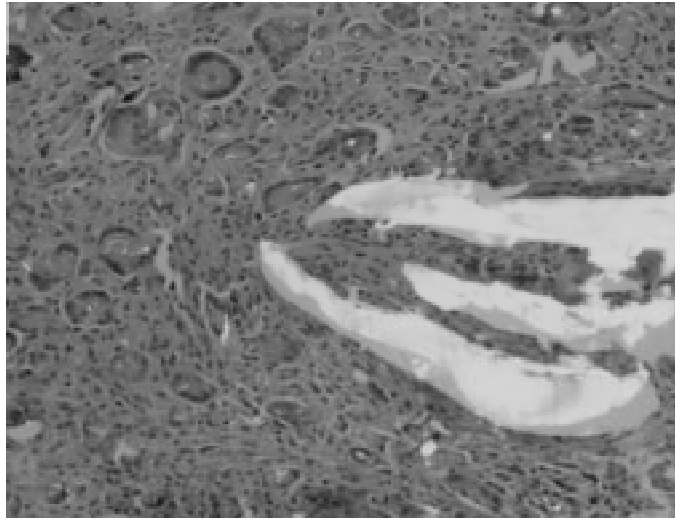


FIG. X2.15 Flakes—Shards

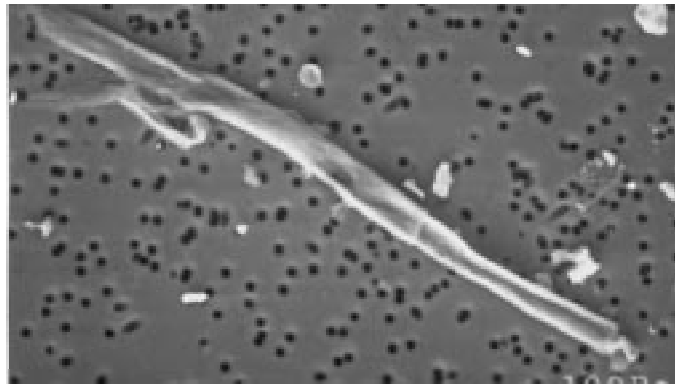


FIG. X2.16 Fibrillar—Straight

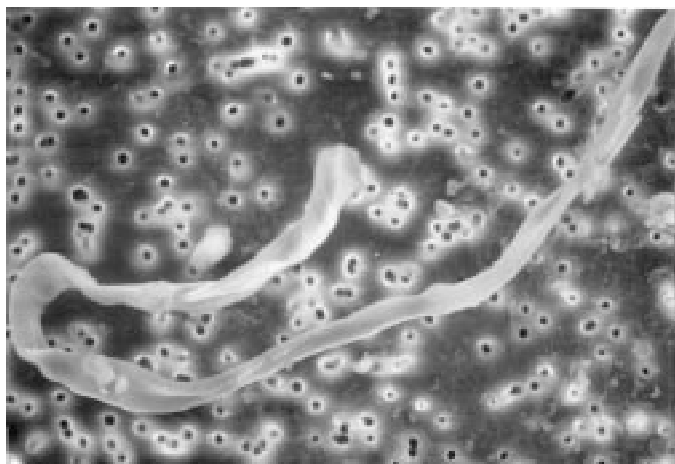


FIG. X2.17 Fibrillar—Twisted

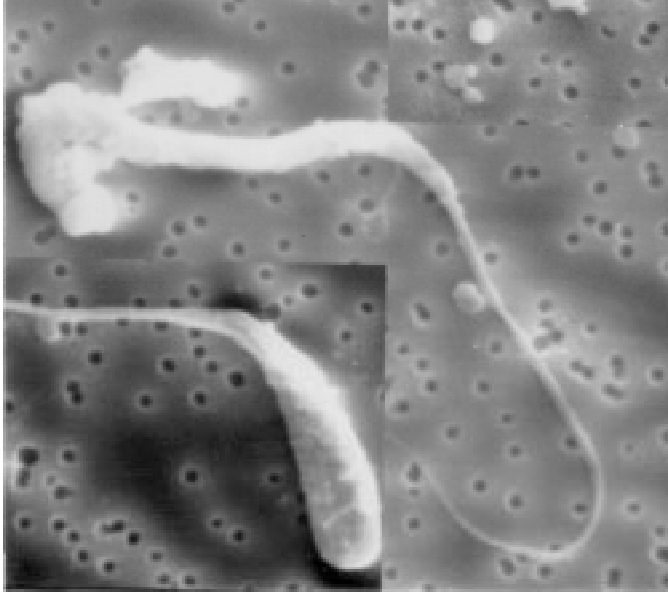


FIG. X2.18 Fibrillar—Seahorse / Hammerhead / Twisted

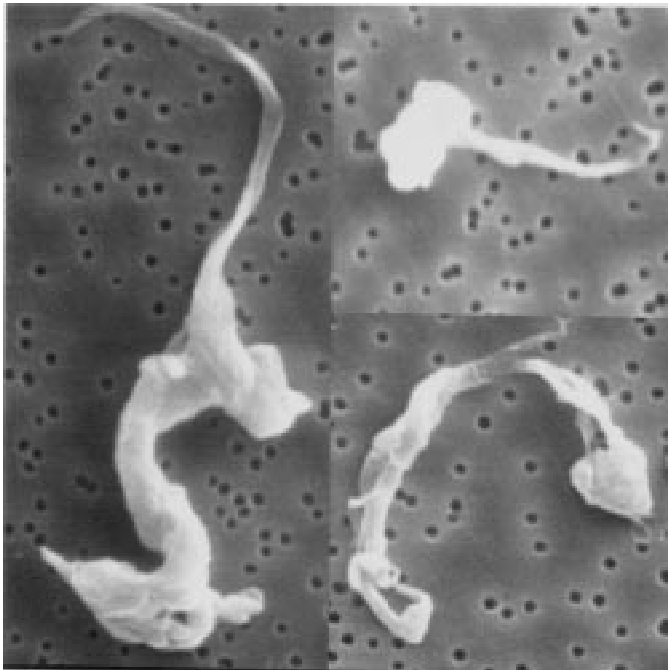


FIG. X2.19 Fibrillar—Hammerhead / Tadpole

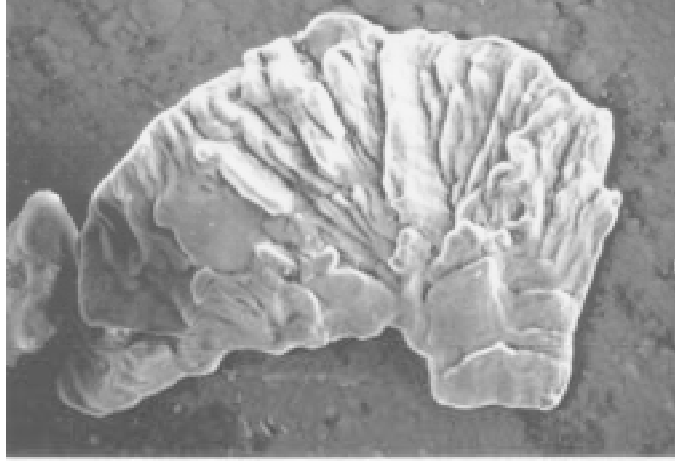


FIG. X2.20 Sharps or Shards—Flakes, Stacked Sheets

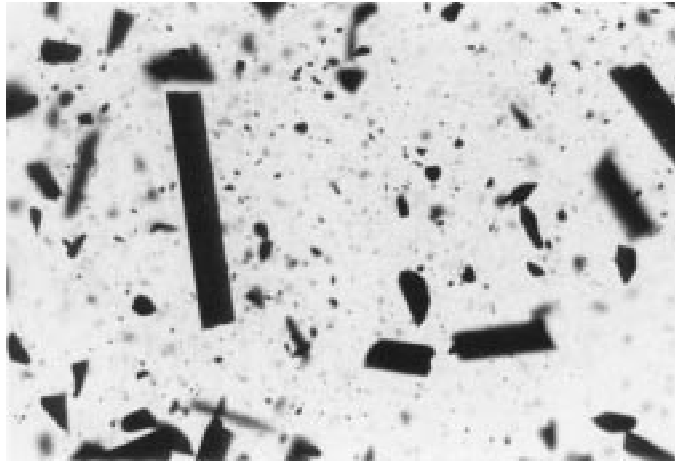


FIG. X2.21 Sharps or Shards—Rectangular Fibers

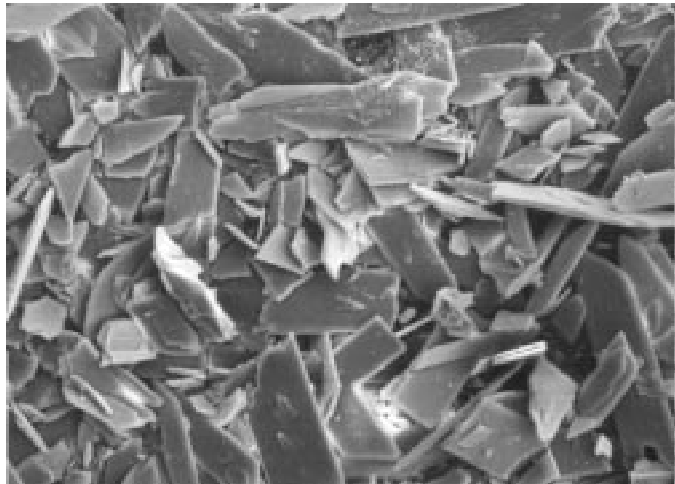


FIG. X2.22 Sharps or Shards—Lathe-Like

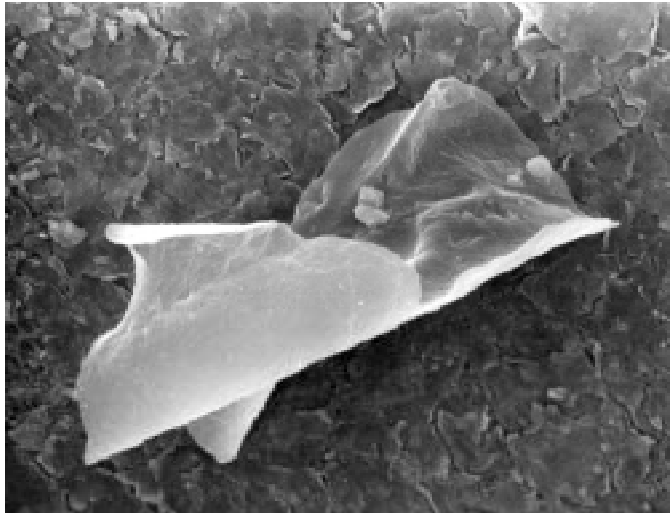


FIG. X2.23 Sharps or Shards—Cuttlefish

X3. RATIONALE

X3.1 Establishment and use of a standardized nomenclature for describing particulate debris is critical for a wide range of studies regarding implants and devices. By using a common vocabulary for particle description, biological responses to different shapes of debris can be separated from other factors such as chemistry. Matching morphology of debris produced in the laboratory with that produced *in vivo* will better refine the accuracy of laboratory test methods. Characterization of debris produced *in vivo* will help in assessment of device performance.

The sample morphologies provided are not intended to be all inclusive of those published in the literature. The intent is to provide illustrative examples of morphologies and to assign names to each type. Thus, communication between investigators should be more precise.

The detailed methods of calculating particle shape have been developed by M. E. Landry and C. M. Agrawal at the University of Texas Health Science Center at San Antonio and are the basis for a Masters of Science in Engineering thesis by M. E. Landry at the University of Texas at Austin. These methods are provided as a way to numerically describe complicated particle shapes. While not all measurements need to be made, standardization of these methods should provide an additional data set for description of the wide variety of particle morphologies generated *in vivo* and *in vitro*.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).