



Standard Specification for Industrial Platinum Resistance Thermometers¹

This standard is issued under the fixed designation E 1137; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last approval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification covers the requirements for metal-sheathed industrial platinum resistance thermometers (PRT's) suitable for direct immersion temperature measurement. It applies to PRT's with an average temperature coefficient of resistance between 0 and 100°C of 0.385 %/°C and nominal resistance at 0°C of 100 Ω or other specified value. This specification covers PRT's suitable for all or part of the temperature range -200 to 650°C. The resistance-temperature relationship and tolerances are specified as well as physical, performance, and testing requirements.

1.2 The values of temperature in this specification are based on the International Temperature Scale of 1990 (ITS-90).²

2. Referenced Documents

2.1 ASTM Standards:

A 269 Specification for Seamless and Welded Austenitic Stainless Steel Tubing for General Service³

B 167 Specification for Nickel-Chromium-Iron Alloys (UNS N06600, N06601, and N06690) Seamless Pipe and Tube⁴

E 344 Terminology Relating to Thermometry and Hydrometry⁵

E 644 Test Methods for Testing Industrial Resistance Thermometers⁵

E 1652 Specification for Magnesium Oxide and Aluminum Oxide Powder and Crushable Insulators Used in the Manufacture of Metal-Sheathed Platinum Resistance Thermometers and Noble Metal Thermocouples⁵

3. Terminology

3.1 *Definitions*—For definitions of terms used in this specification see Terminology E 344.

¹ This specification is under the jurisdiction of ASTM Committee E-20 on Temperature Measurement and is the direct responsibility of Subcommittee E20.03 on Resistance Thermometers.

Current edition approved Nov. 10, 1997. Published May 1998. Originally published as E 1137 – 87. Last previous edition E 1137 – 95.

² Preston-Thomas, H., "The International Temperature Scale of 1990 (ITS-90)," *Metrologia*, Vol 27, No. 1, 1990, pp. 3–10. For errata see *ibid*, Vol 27, No. 2, 1990, p. 107.

³ *Annual Book of ASTM Standards*, Vol 01.01.

⁴ *Annual Book of ASTM Standards*, Vol 02.04.

⁵ *Annual Book of ASTM Standards*, Vol 14.03.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *cable end closure, n*—moisture barrier at the cable end of the sheath.

3.2.2 *connecting wires, n*—wires that run from the element through the cable end closure and external to the sheath.

3.2.2.1 *Discussion*—The closure does not necessarily constitute a hermetic seal.

3.2.3 *excitation, n*—electrical current passing through the element.

3.2.4 *g-level, n*—acceleration of an object relative to the local acceleration of gravity.

3.2.4.1 *Discussion*—For example, a g-level of 5 is equivalent to an acceleration of approximately $5 \times 9.8 \text{ m/s}^2 = 49.0 \text{ m/s}^2$.

3.2.5 *minimum immersion length, n*—depth that a thermometer should be immersed, in a uniform temperature environment, such that further immersion does not produce a change in indicated temperature greater than the specified tolerance.

3.2.6 *PRT design, n*—generic term used to differentiate between different PRT construction details, such as element and connecting wire construction, insulation methods, sealing techniques, and mounting methods (for example, spring loaded or direct mounting).

3.2.7 *self-heating, n*—change in temperature of the element caused by the heating effect of the excitation.

3.2.8 *sheath, n*—cylindrical metal tube with an integral welded closure at the end in which the element is located.

4. Significance and Use

4.1 This specification is written to provide common terminology, resistance versus temperature characteristics, accuracy classification, and inspection requirements for a specified configuration of a typical industrial platinum resistance thermometer (PRT).

4.2 This specification may be used as part of the documentation to support negotiations for the purchase and discussion of such thermometers.

5. Classification of Tolerances

5.1 The PRT shall conform to the resistance-temperature relation (see 9.2.1) within the following tolerances:

$$\text{Grade A} = \pm[0.13 + 0.0017|t|]^\circ\text{C} \quad (1)$$

$$\text{Grade B} = \pm[0.25 + 0.0042 |t|]^\circ\text{C} \quad (2)$$

where:

$|t|$ = value of temperature without regard to sign, °C.

5.1.1 The tolerances are given in Table 1 for a PRT with a nominal resistance of 100 Ω at 0°C.

6. Ordering Information

6.1 The purchase order documents shall specify the following information to ensure that the PRT is adequately described:

- 6.1.1 The number of this specification,
- 6.1.2 Sheath diameter and overall length (see Fig. 1),
- 6.1.3 Sheath material,
- 6.1.4 Minimum and maximum sensed temperature,
- 6.1.5 Maximum temperature at cable end closure,
- 6.1.6 Connection configuration; 2-Wire, 3-Wire, 4-Wire (potentiometric), and compensating loop (4-Wire) (see Fig. 2),
- 6.1.7 Tolerance, (Grade A, or Grade B), and
- 6.1.8 Nominal resistance at 0°C (100 Ω unless otherwise specified).

7. Materials and Manufacture

7.1 All materials used shall be in accordance with the following requirements:

7.1.1 *Sheath Materials*—For temperatures not exceeding 480°C, austenitic stainless steel tubing, conforming to Specification A 269. For temperatures not exceeding 650°C, high-nickel alloy tubing, conforming to Specification B 167.

7.1.2 *Sensing Element*—Sensing element shall be platinum.

7.1.3 *Insulation*—The insulating material within the PRT shall be compatible with the temperature range –200 to 650°C or as specified in 6.1.4. Magnesium oxide (MgO) and aluminum oxide (Al₂O₃) Powders and crushable insulators conforming to Specification E 1652 satisfy this requirement.

7.1.4 *Cable End Potting Materials*—Potting materials shall provide a barrier against water and other liquids and generally prevent the penetration of water vapor. Any potting material used shall be compatible with the ambient temperatures specified for the application.

NOTE 1—Typically, epoxy materials are used for ambient temperatures less than 200°C and moisture impervious ceramic adhesives are used over 200°C, but the cable end potting shall not be limited to these materials if the end seal meets all other requirements of this specification.

TABLE 1 Classification Tolerances^{A, B}

Temperature, <i>t</i> , °C	Grade A		Grade B	
	°C	Ω	°C	Ω
–200	0.47	0.20	1.1	0.47
–100	0.30	0.12	0.67	0.27
0	0.13	0.05	0.25	0.10
100	0.30	0.11	0.67	0.25
200	0.47	0.17	1.1	0.40
300	0.64	0.23	1.5	0.53
400	0.81	0.28	1.9	0.66
500	0.98	0.33	2.4	0.78
600	1.15	0.37	2.8	0.88
650	1.24	0.40	3.0	0.94

^A The table represents values for 3-wire and 4-wire PRT's. Caution must be exercised with 2-wire PRT's because of possible errors caused by connecting wires.

^B Tabulated values are based on elements of 100.0 Ω (nominal) at 0°C.

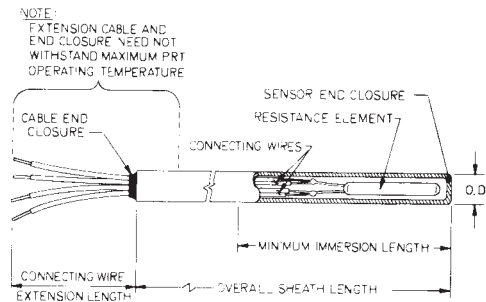


FIG. 1 Platinum Resistance Thermometer

7.1.5 *Connecting Wires*—Typically, materials of connecting wires are: nickel plated copper, nickel, platinum, constantan, or manganin. Any material used in joining the connecting wires to the PRT element must withstand the maximum operating temperature of the PRT.

8. Other Requirements

8.1 *Pressure*—The PRT shall withstand an external pressure of 21 MPa (3000 psig) and shall be tested in accordance with Test Methods E 644 pressure test. The PRT shall remain within the tolerance specified in 5.1.

8.2 *Vibration*:

8.2.1 The PRT shall withstand vibration testing as described in Test Methods E 644 using the test in Table 2.

8.2.2 The PRT shall be mounted by installation in the thermowell or by threaded connection to simulate normal mounting procedure as limited by Table 2.

8.2.3 The PRT shall be continuously energized with an oscilloscope-monitored 1.0-mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

8.2.4 After the PRT is tested for vibration the insulation resistance of the PRT shall remain within the tolerance of Table 3 and the resistance at 0°C within the tolerance specified in 5.1.

8.3 *Mechanical Shock*:

8.3.1 The PRT shall withstand mechanical shock testing as described in Test Methods E 644. The half-sine pulse shall have a peak *g*-level of 50 and duration of 11 ms.

8.3.2 The PRT shall be continuously energized with an oscilloscope-monitored 1.0-mA dc excitation. There shall be no discontinuity of the monitored trace during the test.

8.3.3 After the PRT is tested for mechanical shock the insulation resistance of the PRT shall remain with the tolerance of Table 3 and the resistance at 0°C within the tolerance in 5.1.

8.4 *Thermal*:

8.4.1 The PRT shall be capable of continuous operation over the specified temperature range (see 6.1).

8.4.2 The cable end closure and external connecting wires need not withstand the maximum PRT operating temperature.

9. Performance

9.1 *Excitation*:

9.1.1 The PRT must be constructed such that it is usable in ac or dc measurement systems. In ac measuring systems, reactance effects shall be considered.

9.1.2 The PRT shall be capable of operating with continuous excitation of 10 mA. However, excitation of 1 mA or less is

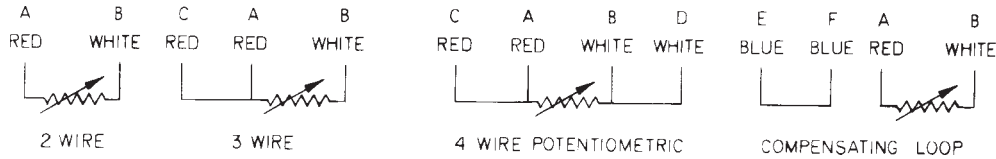


FIG. 2 Connection Configurations

TABLE 2 Vibration Test Parameters

NOTE 1— The values in Table 2 apply to a PRT mounted in a thermowell with nominal clearance of less than 0.25 mm (0.01 in.) in diameter. If the PRT is not mounted in a thermowell, the values in Table 2 apply to a PRT with an unsupported stem length less than 102 mm (4 in.).

Frequency	5 to 500 Hz
Test Level	1.27-mm (0.05-in.) double amplitude displacement or peak g-level of 3, whichever is less
Resonant Dwell Time	30 min for each resonant point
Cycling Time	3 h per axis less the time spent at resonant dwells at the axis.
Mounting	As normally mounted including the mating thermowell, if applicable.

TABLE 3 Insulation Resistance

Applied dc Voltage, Volts dc		Minimum Insulation Resistance	
min	max	°C	MΩ
10	50	25 ± 5	100
10	50	300 ± 10	10
10	50	650 ± 15	2

recommended to minimize measurement errors associated with self-heating (see 9.4).

9.2 Resistance versus Temperature Relation:

9.2.1 Resistance-Temperature Equations—Within the specified tolerances (see 5.1), the PRT shall have resistance-temperature characteristics defined as follows:

for the range $-200^{\circ}\text{C} \leq t < 0^{\circ}\text{C}$:

$$R_t = R_o [1 + At + Bt^2 + C(t - 100)t^3] \Omega \tag{3}$$

for the range $0^{\circ}\text{C} \leq t \leq 650^{\circ}\text{C}$:

$$R_t = R_o [1 + At + Bt^2] \Omega \tag{4}$$

where:

- t = temperature (ITS-90), °C,
- R_t = resistance at temperature (t),
- R_o = resistance at 0°C,
- $A = 3.9083 \times 10^{-3} \text{ }^{\circ}\text{C}^{-1}$,
- $B = -5.775 \times 10^{-7} \text{ }^{\circ}\text{C}^{-2}$, and
- $C = -4.183 \times 10^{-12} \text{ }^{\circ}\text{C}^{-4}$.

9.2.2 Resistance Table—Resistance values of the PRT versus temperature using the equations of 9.2.1 and R_o of 100 Ω are given in Table 4.

NOTE 2—The resistance versus temperature relationship for a specific thermometer may be computed from measured resistance of that specific thermometer.

9.2.3 Inverse equations that may be used to compute values of temperature (°C) as a function of resistance are given in Appendix X1.

9.3 Insulation Resistance—The insulation resistance between each connecting wire and the sheath shall meet the

requirements of Table 3 when tested in accordance with Test Methods E 644. The PRT shall be tested with at least the minimum immersion length exposed to the temperature environment.

9.4 Self-Heating—A power of at least 33 mW shall be required to produce a self-heating of 1°C when the PRT is tested in water in accordance with Test Methods E 644.

9.5 Thermal Response Time—The 63.2 % response time shall not exceed the values in Table 5 when determined in accordance with Test Methods E 644. The step change in temperature shall be from $20 \pm 5^{\circ}\text{C}$ air to $77 \pm 5^{\circ}\text{C}$ water flowing at $0.9 \pm 0.09 \text{ m/s}$ ($3.0 \pm 0.3 \text{ ft/s}$).

9.6 Thermoelectric Effect—Wire connections between the PRT sensing element, inner connecting wires, and external connecting wires can generate small voltages when these connection points are exposed to different temperatures. This thermoelectric voltage can add or subtract from the voltage measured across a PRT and cause an unknown variable error in measurement. When tested in accordance with Test Methods E 644, the PRT shall remain within the tolerances specified in 5.1 with an excitation of 1-mA dc, regardless of polarity.

9.7 Stability—When tested in accordance with Test Methods E 644, the PRT shall remain within the tolerances specified in 5.1 for a four-week test. During this test, the resistance at 0°C shall be checked at regular intervals (2 times per week).

9.8 Minimum Immersion Length—When determined in accordance with Test Methods E 644, the PRT minimum immersion length shall be less than 51 mm (2 in.). The limit of uncertainty shall be 0.13°C and 0.25°C for Grade A and Grade B PRT’s respectively.

10. Dimensions, Mass, and Permissible Variations

10.1 A PRT without a process fitting or other means of attachment is shown in Fig. 1.

10.2 PRT’s manufactured in accordance with this specification shall be able to pass through the straightness ring gage with the gage sizes listed in Table 6.

11. Required Tests

11.1 Qualification Tests—The PRT shall be subjected to the tests outlined in Table 7 to demonstrate conformance to this specification. The manufacturer shall perform these tests at least one time to qualify the PRT design. Thereafter, it is recommended these tests be used on a periodic basis to verify process control.

11.1.1 Qualification Test Report—The manufacturer shall prepare and retain a qualification test report applicable to the PRT design that documents the model number, test procedure (by reference to Test Methods E 644 and this specification), and the results obtained.

TABLE 4 Resistance versus Temperature^{A, B}

ITS-90° C	0	-1	-2	-3	-4	-5	-6	-7	-8	-9	-10
-200	18.52										
-190	22.83	22.40	21.97	21.54	21.11	20.68	20.25	19.82	19.38	18.95	18.52
-180	27.10	26.67	26.24	25.82	25.39	24.97	24.54	24.11	23.68	23.25	22.83
-170	31.34	30.91	30.49	30.07	29.64	29.22	28.80	28.37	27.95	27.52	27.10
-160	35.54	35.12	34.70	34.28	33.86	33.44	33.02	32.60	32.18	31.76	31.34
-150	39.72	39.31	38.89	38.47	38.05	37.64	37.22	36.80	36.38	35.96	35.54
-140	43.88	43.46	43.05	42.63	42.22	41.80	41.39	40.97	40.56	40.14	39.72
-130	48.00	47.59	47.18	46.77	46.36	45.94	45.53	45.12	44.70	44.29	43.88
-120	52.11	51.70	51.29	50.88	50.47	50.06	49.65	49.24	48.83	48.42	48.00
-110	56.19	55.79	55.38	54.97	54.56	54.15	53.75	53.34	52.93	52.52	52.11
-100	60.26	59.85	59.44	59.04	58.63	58.23	57.82	57.41	57.01	56.60	56.19
-90	64.30	63.90	63.49	63.09	62.68	62.28	61.88	61.47	61.07	60.66	60.26
-80	68.33	67.92	67.52	67.12	66.72	66.31	65.91	65.51	65.11	64.70	64.30
-70	72.33	71.93	71.53	71.13	70.73	70.33	69.93	69.53	69.13	68.73	68.33
-60	76.33	75.93	75.53	75.13	74.73	74.33	73.93	73.53	73.13	72.73	72.33
-50	80.31	79.91	79.51	79.11	78.72	78.32	77.92	77.52	77.12	76.73	76.33
-40	84.27	83.87	83.48	83.08	82.69	82.29	81.89	81.50	81.10	80.70	80.31
-30	88.22	87.83	87.43	87.04	86.64	86.25	85.85	85.46	85.06	84.67	84.27
-20	92.16	91.77	91.37	90.98	90.59	90.19	89.80	89.40	89.01	88.62	88.22
-10	96.09	95.69	95.30	94.91	94.52	94.12	93.73	93.34	92.95	92.55	92.16
0	100.00	99.61	99.22	98.83	98.44	98.04	97.65	97.26	96.87	96.48	96.09
ITS-90° C	0	1	2	3	4	5	6	7	8	9	10
0	100.00	100.39	100.78	101.17	101.56	101.95	102.34	102.73	103.12	103.51	103.90
10	103.90	104.29	104.68	105.07	105.46	105.85	106.24	106.63	107.02	107.40	107.79
20	107.79	108.18	108.57	108.96	109.35	109.73	110.12	110.51	110.90	111.29	111.67
30	111.67	112.06	112.45	112.83	113.22	113.61	114.00	114.38	114.77	115.15	115.54
40	115.54	115.93	116.31	116.70	117.08	117.47	117.86	118.24	118.63	119.01	119.40
50	119.40	119.78	120.17	120.55	120.94	121.32	121.71	122.09	122.47	122.86	123.24
60	123.24	123.63	124.01	124.39	124.78	125.16	125.54	125.93	126.31	126.69	127.08
70	127.08	127.46	127.84	128.22	128.61	128.99	129.37	129.75	130.13	130.52	130.90
80	130.90	131.28	131.66	132.04	132.42	132.80	133.18	133.57	133.95	134.33	134.71
90	134.71	135.09	135.47	135.85	136.23	136.61	136.99	137.37	137.75	138.13	138.51
100	138.51	138.88	139.26	139.64	140.02	140.40	140.78	141.16	141.54	141.91	142.29
110	142.29	142.67	143.05	143.43	143.80	144.18	144.56	144.94	145.31	145.69	146.07
120	146.07	146.44	146.82	147.20	147.57	147.95	148.33	148.70	149.08	149.46	149.83
130	149.83	150.21	150.58	150.96	151.33	151.71	152.08	152.46	152.83	153.21	153.58
140	153.58	153.96	154.33	154.71	155.08	155.46	155.83	156.20	156.58	156.95	157.33
150	157.33	157.70	158.07	158.45	158.82	159.19	159.56	159.94	160.31	160.68	161.05
160	161.05	161.43	161.80	162.17	162.54	162.91	163.29	163.66	164.03	164.40	164.77
170	164.77	165.14	165.51	165.89	166.26	166.63	167.00	167.37	167.74	168.11	168.48
180	168.48	168.85	169.22	169.59	169.96	170.33	170.70	171.07	171.43	171.80	172.17
190	172.17	172.54	172.91	173.28	173.65	174.02	174.38	174.75	175.12	175.49	175.86
200	175.86	176.22	176.59	176.96	177.33	177.69	178.06	178.43	178.79	179.16	179.53
210	179.53	179.89	180.26	180.63	180.99	181.36	181.72	182.09	182.46	182.82	183.19
220	183.19	183.55	183.92	184.28	184.65	185.01	185.38	185.74	186.11	186.47	186.84
230	186.84	187.20	187.56	187.93	188.29	188.66	189.02	189.38	189.75	190.11	190.47
240	190.47	190.84	191.20	191.56	191.92	192.29	192.65	193.01	193.37	193.74	194.10
250	194.10	194.46	194.82	195.18	195.55	195.91	196.27	196.63	196.99	197.35	197.71
260	197.71	198.07	198.43	198.79	199.15	199.51	199.87	200.23	200.59	200.95	201.31
270	201.31	201.67	202.03	202.39	202.75	203.11	203.47	203.83	204.19	204.55	204.90
280	204.90	205.26	205.62	205.98	206.34	206.70	207.05	207.41	207.77	208.13	208.48
290	208.48	208.84	209.20	209.56	209.91	210.27	210.63	210.98	211.34	211.70	212.05
300	212.05	212.41	212.76	213.12	213.48	213.83	214.19	214.54	214.90	215.25	215.61
310	215.61	215.96	216.32	216.67	217.03	217.38	217.74	218.09	218.44	218.80	219.15
320	219.15	219.51	219.86	220.21	220.57	220.92	221.27	221.63	221.98	222.33	222.68
330	222.68	223.04	223.39	223.74	224.09	224.45	224.80	225.15	225.50	225.85	226.21
340	226.21	226.56	226.91	227.26	227.61	227.96	228.31	228.66	229.01	229.37	229.72
350	229.72	230.07	230.42	230.77	231.12	231.47	231.82	232.17	232.52	232.87	233.21
360	233.21	233.56	233.91	234.26	234.61	234.96	235.31	235.66	236.01	236.35	236.70
370	236.70	237.05	237.40	237.74	238.09	238.44	238.79	239.13	239.48	239.83	240.18
380	240.18	240.52	240.87	241.22	241.56	241.91	242.26	242.60	242.95	243.29	243.64
390	243.64	243.99	244.33	244.68	245.02	245.37	245.71	246.06	246.40	246.75	247.09
400	247.09	247.44	247.78	248.13	248.47	248.81	249.15	249.50	249.85	250.19	250.53
410	250.53	250.88	251.22	251.56	251.91	252.25	252.59	252.93	253.28	253.62	253.96
420	253.96	254.30	254.65	254.99	255.33	255.67	256.01	256.35	256.70	257.04	257.38
430	257.38	257.72	258.06	258.40	258.74	259.08	259.42	259.76	260.10	260.44	260.78
440	260.78	261.12	261.46	261.80	262.14	262.48	262.82	263.16	263.50	263.84	264.18
450	264.18	264.52	264.86	265.20	265.53	265.87	266.21	266.55	266.89	267.22	267.56
460	267.56	267.90	268.24	268.57	268.91	269.25	269.59	269.92	270.26	270.60	270.93
470	270.93	271.27	271.61	271.94	272.28	272.61	272.95	273.29	273.62	273.96	274.29

TABLE 4 *Continued*

ITS-90° C	0	1	2	3	4	5	6	7	8	9	10
480	274.29	274.63	274.96	275.30	275.63	275.97	276.30	276.64	276.97	277.31	277.64
490	277.64	277.98	278.31	278.64	278.98	279.31	279.64	279.98	280.31	280.64	280.98
500	280.98	281.31	281.64	281.98	282.31	282.64	282.97	283.31	283.64	283.97	284.30
510	284.30	284.63	284.97	285.30	285.63	285.96	286.29	286.62	286.95	287.29	287.62
520	287.62	287.95	288.28	288.61	288.94	289.27	289.60	289.93	290.26	290.59	290.92
530	290.92	291.25	291.58	291.91	292.24	292.56	292.89	293.22	293.55	293.88	294.21
540	294.21	294.54	294.86	295.19	295.52	295.85	296.18	296.50	296.83	297.16	297.49
550	297.49	297.81	298.14	298.47	298.80	299.12	299.45	299.78	300.10	300.43	300.75
560	300.75	301.08	301.41	301.73	302.06	302.38	302.71	303.03	303.36	303.69	304.01
570	304.01	304.34	304.66	304.98	305.31	305.63	305.96	306.28	306.61	306.93	307.25
580	307.25	307.58	307.90	308.23	308.55	308.87	309.20	309.52	309.84	310.16	310.49
590	310.49	310.81	311.13	311.45	311.78	312.10	312.42	312.74	313.06	313.39	313.71
600	313.71	314.03	314.35	314.67	314.99	315.31	315.64	315.96	316.28	316.60	316.92
610	316.92	317.24	317.56	317.88	318.20	318.52	318.84	319.16	319.48	319.80	320.12
620	320.12	320.43	320.75	321.07	321.39	321.71	322.03	322.35	322.67	322.98	323.30
630	323.30	323.62	323.94	324.26	324.57	324.89	325.21	325.53	325.84	326.16	326.48
640	326.48	326.79	327.11	327.43	327.74	328.06	328.38	328.69	329.01	329.32	329.64
650	329.64										

^A This table is based on the equations of 9.2.1 and R_o of 100 Ω . For PRT's with R_o values other than 100 Ω , the resistance-temperature characteristics can be calculated using the equations of 9.2.1 or by multiplying the tabulated values of resistance by the ratio $R_o/100$.

^B Temperature is expressed in degrees Celsius (ITS-90). To determine the temperature corresponding to a tabulated value of resistance, first locate the decade temperature left of the resistance value. To this temperature, add the temperature increment located above the resistance value. For example, the resistance values of 84.67, 187.56, and 253.96 Ω correspond to temperatures of – 39, 232, and 420°C respectively.

TABLE 5 Thermal Response Time

Sheath Outside Diameter		63.2 % Step Response Time
in.	mm	s
0.125	3.2	3
0.250	6.4	8

TABLE 6 Dimensions and Tolerances

Sheath Sizes				Straightness Ring Cage			
Diameter		Tolerance		Length		Inside Diameter	
in.	mm	± in.	± mm	in.	mm	in.	mm
0.125	3.18	0.004	0.1	1.3	33	0.131	3.33
0.250	6.35	0.004	0.1	2.5	64	0.256	6.50

TABLE 7 Required Tests

Test	Test Methods E 644, Section	Acceptance Criteria, Specification E 1137, Paragraph
Insulation Resistance	5	9.3
Resistance versus Temperature	6	9.2
Minimum Immersion Length	7	9.8
Pressure	8	8.1
Thermal Response Time	9	9.5
Vibration	10	8.2
Self-Heating	12	9.4
Stability	13	9.7
Thermoelectric Effect	14	9.6
Mechanical Shock	11	8.3
Dimensional	N/A	10.2

11.2 *Acceptance Tests*—The manufacturer shall verify that the PRT to be delivered satisfies the following minimum test requirements: resistance at 0°C (see 5.1), room temperature insulation resistance (see 9.3), and dimensions (see 10.2).

NOTE 3—The purchaser may perform any of the tests included in Table 7 as a basis for acceptance or rejection.

12. Declaration of Conformity

12.1 The manufacturer shall provide a document to the purchaser that states the PRT satisfies the requirements of this specification.

13. Product Marking

13.1 Each PRT shall carry a permanent marking that identifies the producer, grade, serial number, and this ASTM designation.

14. Packaging

14.1 Each PRT shall be packaged to adequately protect it against handling shock and vibration in transportation and storage.

15. Keywords

15.1 ITS-90; metal sheath; platinum resistance thermometer; PRT

APPENDIX

(Nonmandatory Information)

X1. TEMPERATURE VERSUS RESISTANCE EQUATIONS

X1.1 The following inverse equations may be used to compute values of temperature ($^{\circ}\text{C}$) as a function of resistance over the range of -200 to 650°C . The computed values of temperature will be within the tolerances of 5.1 plus the error, if any, associated with the inverse equation.

For $R_t/R_o < 1$ ($t < 0^{\circ}\text{C}$), an approximate inverse of Eq 3 within $\pm 0.002^{\circ}\text{C}$ is:

$$t = \sum_{i=1}^4 D_i (R_t/R_o - 1)^i \quad (\text{X1.1})$$

For $R_t/R_o \geq 1$ ($t \geq 0^{\circ}\text{C}$), the inverse of Eq 4 is:

$$t = \frac{\sqrt{A^2 - 4B(1 - R_t/R_o)} - A}{2B} \quad (\text{X1.2})$$

where:

- t = temperature ITS-90, $^{\circ}\text{C}$
- R_t = resistance at temperature t , Ω ,
- R_o = resistance at 0°C , Ω ,
- A = $3.9083 \times 10^{-3} \text{ }^{\circ}\text{C}^{-1}$
- B = $-5.775 \times 10^{-7} \text{ }^{\circ}\text{C}^{-2}$,
- D_1 = 255.819°C ,
- D_2 = 9.14550°C ,
- D_3 = -2.92363°C , and
- D_4 = 1.79090°C .

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).