



## Standard Test Method for Dynamic Young's Modulus, Shear Modulus, and Poisson's Ratio for Advanced Ceramics by Sonic Resonance<sup>1</sup>

This standard is issued under the fixed designation C 1198; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

### 1. Scope

1.1 This test method covers the determination of the dynamic elastic properties of advanced ceramics. Specimens of these materials possess specific mechanical resonant frequencies that are determined by the elastic modulus, mass, and geometry of the test specimen. Therefore, the dynamic elastic properties of a material can be computed if the geometry, mass, and mechanical resonant frequencies of a suitable test specimen of that material can be measured. Dynamic Young's modulus is determined using the resonant frequency in the flexural mode of vibration. The dynamic shear modulus, or modulus of rigidity, is found using torsional resonant vibrations. Dynamic Young's modulus and dynamic shear modulus are used to compute Poisson's ratio.

1.2 This test method is specifically appropriate for advanced ceramics that are elastic, homogeneous, and isotropic (**1**).<sup>2</sup> Advanced ceramics of a composite character (particulate, whisker, or fiber reinforced) may be tested by this test method with the understanding that the character (volume fraction, size, morphology, distribution, orientation, elastic properties, and interfacial bonding) of the reinforcement in the test specimen will have a direct effect on the elastic properties. These reinforcement effects must be considered in interpreting the test results for composites. This test method is not satisfactory for specimens that have cracks or voids that are major discontinuities in the specimen. Neither is the test method satisfactory when these materials cannot be fabricated in a uniform rectangular or circular cross section.

1.3 A high-temperature furnace and cryogenic cabinet are described for measuring the dynamic elastic moduli as a function of temperature from  $-195$  to  $1200^{\circ}\text{C}$ .

1.4 Modification of this test method for use in quality control is possible. A range of acceptable resonant frequencies is determined for a specimen with a particular geometry and mass. Any specimen with a frequency response falling outside this frequency range is rejected. The actual modulus of each specimen need not be determined as long as the limits of the

selected frequency range are known to include the resonant frequency that the specimen must possess if its geometry and mass are within specified tolerances.

1.5 The procedures in this test method are, where possible, consistent with the procedures of Test Methods C 623, C 747, and C 848. The tables of these test methods have been replaced by the actual formulas from the original references. With the advent of computers and sophisticated hand calculators, the actual formulas can be easily used and provide greater accuracy than factor tables.

1.6 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

### 2. Referenced Documents

#### 2.1 ASTM Standards:

- C 372 Test Method for Linear Thermal Expansion of Porcelain Enamel and Glaze Frits and Fired Ceramic Whiteware Products by the Dilatometer Method<sup>3</sup>
- C 623 Test Method for Young's Modulus, Shear Modulus, and Poisson's Ratio for Glass and Glass-Ceramics by Resonance<sup>3</sup>
- C 747 Test Method for Moduli of Elasticity and Fundamental Frequencies of Carbon and Graphite Materials by Sonic Resonance<sup>4</sup>
- C 848 Test Method for Young's Modulus, Shear Modulus, and Poisson's Ratio for Ceramic Whitewares by Resonance<sup>3</sup>
- C 1145 Terminology of Advanced Ceramics<sup>4</sup>
- C 1161 Test Method for Flexural Strength of Advanced Ceramics at Ambient Temperatures<sup>4</sup>
- D 4092 Terminology Relating to Dynamic Mechanical Measurements on Plastics<sup>5</sup>

### 3. Terminology

#### 3.1 Definitions:

<sup>3</sup> Annual Book of ASTM Standards, Vol 15.02.

<sup>4</sup> Annual Book of ASTM Standards, Vol 15.01.

<sup>5</sup> Annual Book of ASTM Standards, Vol 08.02.

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee C-28 on Advanced Ceramics and is the direct responsibility of Subcommittee C28.01 on Properties and Performance.

Current edition approved June 10, 1996. Published August 1996. Originally published as C 1198 – 91. Last previous edition C 1198 – 91.

<sup>2</sup> The boldface numbers given in parentheses refer to a list of references at the end of the text.

3.1.1 *advanced ceramic, n*—a highly engineered, high performance, predominately nonmetallic, inorganic, ceramic material having specific functional attributes. (C 1145)

3.1.2 *dynamic mechanical measurement, n*—a technique in which either the modulus or damping, or both, of a substance under oscillatory load or displacement is measured as a function of temperature, frequency, or time, or combination thereof. (D 4092)

3.1.3 *elastic limit* [FL<sup>-2</sup>], *n*—the greatest stress that a material is capable of sustaining without permanent strain remaining upon complete release of the stress.

3.1.4 *elastic modulus* [FL<sup>-2</sup>], *n*—the ratio of stress to strain below the proportional limit.

3.1.5 *Poisson's ratio* ( $\mu$ ) [nd], *n*—the absolute value of the ratio of transverse strain to the corresponding axial strain resulting from uniformly distributed axial stress below the proportional limit of the material.

3.1.6 *Discussion*—In isotropic materials Young's modulus ( $E$ ), shear modulus ( $G$ ), and Poisson's ratio ( $\mu$ ) are related by the following equation:

$$\mu = (E/2G) - 1 \quad (1)$$

3.1.7 *proportional limit* [FL<sup>-2</sup>], *n*—the greatest stress that a material is capable of sustaining without deviation from proportionality of stress to strain (Hooke's law).

3.1.8 *shear modulus* ( $G$ ) [FL<sup>-2</sup>], *n*—the elastic modulus in shear or torsion. Also called *modulus of rigidity* or *torsional modulus*.

3.1.9 *Young's modulus* ( $E$ ) [FL<sup>-2</sup>], *n*—the elastic modulus in tension or compression.

### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 *anti-nodes, n*—an unconstrained slender rod or bar in resonance contains two or more locations that have local maximum displacements, called anti-nodes. For the fundamental flexure resonance, the anti-nodes are located at the two ends and the center of the specimen.

3.2.2 *elastic, adj*—the property of a material such that an application of stress within the elastic limit of that material making up the body being stressed will cause an instantaneous and uniform deformation, that will be eliminated upon removal of the stress, with the body returning instantly to its original size and shape without energy loss. Most advanced ceramics conform to this definition well enough to make this resonance test valid.

3.2.3 *flexural vibrations, n*—the vibrations that occur when the oscillations in a slender rod or bar are in the plane normal to the length dimension.

3.2.4 *homogeneous, adj*—the condition of a specimen such that the composition and density are uniform, such that any smaller specimen taken from the original is representative of the whole. Practically, as long as the geometrical dimensions of the test specimen are large with respect to the size of individual grains, crystals, or components, the body can be considered homogeneous.

3.2.5 *isotropic, adj*—the condition of a specimen such that the values of the elastic properties are the same in all directions in the material. Advanced ceramics are considered isotropic on a macroscopic scale, if they are homogeneous and there is a

random distribution and orientation of phases, crystallites, and components.

3.2.6 *nodes, n*—a slender rod or bar in resonance contains one or more locations having a constant zero displacement, called nodes. For the fundamental flexural resonance, the nodes are located at 0.224  $L$  from each end, where  $L$  is the length of the specimen.

3.2.7 *resonance, n*—a slender rod or bar driven into one of the modes of vibration described in 3.2.3 or 3.2.9 is said to be in resonance when the imposed frequency is such that the resultant displacements for a given amount of driving force are at a maximum. The resonant frequencies are natural vibration frequencies that are determined by the elastic modulus, mass, and dimensions of the test specimen.

3.2.8 *slender rod or bar, n*—in dynamic elastic property testing, a specimen whose ratio of length to minimum cross-sectional dimension is at least five and preferably in the range of 20 to 25.

3.2.9 *torsional vibrations, n*—the vibrations that occur when the oscillations in each cross-sectional plane of a slender rod or bar are such that the plane twists around the length dimension axis.

## 4. Summary of Test Method

4.1 This test method measures the resonant frequencies of test specimens of suitable geometry by exciting them at continuously variable frequencies. Mechanical excitation of the bars is provided through the use of a transducer that transforms a cyclic electrical signal into a cyclic mechanical force on the specimen. A second transducer senses the resulting mechanical vibrations of the specimen and transforms them into an electrical signal. The amplitude and frequency of the signal are measured by an oscilloscope or other means to detect resonance. The resonant frequencies, dimensions, and mass of the specimen are used to calculate dynamic Young's modulus and dynamic shear modulus.

## 5. Significance and Use

5.1 This test method may be used for material development, characterization, design data generation, and quality control purposes. It is specifically appropriate for determining the modulus of advanced ceramics that are elastic, homogeneous, and isotropic.

5.1.1 This test method is nondestructive in nature. Only minute stresses are applied to the specimen, thus minimizing the possibility of fracture.

5.1.2 The period of time during which measurement stress is applied and removed is of the order of hundreds of microseconds. With this test method it is feasible to perform measurements at high temperatures, where delayed elastic and creep effects would invalidate modulus measurements calculated from static loading.

5.2 This test method has advantages in certain respects over the use of static loading systems for measuring moduli in advanced ceramics. It is nondestructive in nature and can be used for specimens prepared for other tests. Specimens are subjected to minute strains; hence, the moduli are measured at or near the origin of the stress-strain curve with the minimum possibility of fracture. The period of time during which

measurement stress is applied and removed is of the order of hundreds of microseconds. With this test method it is feasible to perform measurements at high temperatures, where delayed elastic and creep effects would invalidate modulus measurements calculated from static loading.

## 6. Interferences

6.1 The relationships between resonant frequency and dynamic modulus presented herein are specifically applicable to homogeneous, elastic, isotropic materials.

6.1.1 This test method of determining the moduli is applicable to composite ceramics and inhomogeneous materials only with careful consideration of the effect of inhomogeneities and anisotropy. The character (volume fraction, size, morphology, distribution, orientation, elastic properties, and interfacial bonding) of the reinforcement/inhomogeneities in the specimens will have a direct effect on the elastic properties of the specimen as a whole. These effects must be considered in interpreting the test results for composites and inhomogeneous materials.

6.1.2 If specific surface treatments (coatings, machining, grinding, etching, etc.) change the elastic properties of the near-surface material, there will be accentuated effects on the properties measured by this flexural method, as compared to static/bulk measurements by tensile or compression testing.

6.1.3 This test method is not satisfactory for specimens that have major discontinuities, such as large cracks (internal or surface) or voids.

6.2 This test method for determining moduli is limited to specimens with regular geometries (rectangular parallelepiped and cylinders) for which analytical equations are available to relate geometry, mass, and modulus to the resonant vibration frequencies. This test method is not appropriate for determining the elastic properties of materials which cannot be fabricated into such geometries.

6.2.1 The analytical equations assume parallel/concentric dimensions for the regular geometries of the specimen. Deviations from the specified tolerances for the dimensions of the specimens will change the resonant frequencies and introduce error into the calculations.

6.2.2 Edge treatments such as chamfers or radii are not considered in the analytical equations. Edge chamfers on flexure bars prepared according to Test Method C 1161 will change the resonant frequency of the test bars and introduce error into the calculations of the dynamic modulus. It is recommended that specimens for this test not have chamfered or rounded edges.

6.2.3 For specimens with as-fabricated/rough or uneven surfaces, variations in dimension can have a significant effect in the calculations. For example, in the calculation of the dynamic modulus, the modulus value is inversely proportional to the cube of the thickness. Uniform specimen dimensions and precise measurements are essential for accurate results.

## 7. Apparatus

7.1 The test apparatus is shown in Fig. 1. It consists of a variable-frequency audio oscillator, used to generate a sinusoidal voltage, and a power amplifier and suitable transducer to convert the electrical signal to a mechanical driving vibration.

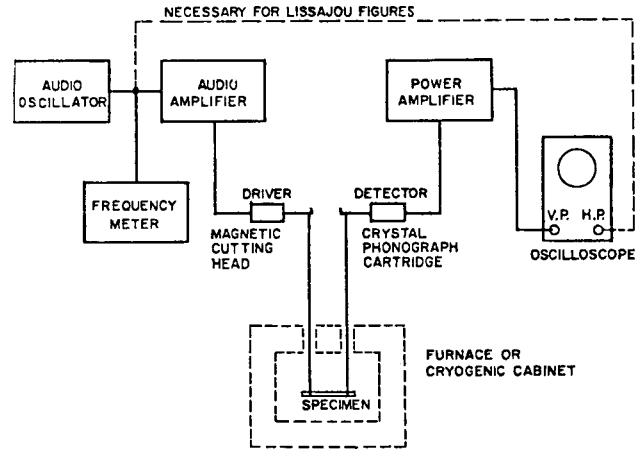


FIG. 1 Block Diagram of a Typical Test Apparatus

A frequency meter (preferably digital) monitors the audio oscillator output to provide an accurate frequency determination. A suitable suspension-coupling system supports the test specimen. Another transducer acts to detect mechanical vibration in the specimen and to convert it into an electrical signal that is passed through an amplifier and displayed on an indicating meter. The meter may be a voltmeter, microammeter, or oscilloscope. An oscilloscope is recommended because it enables the operator to positively identify resonances, including higher order harmonics, by Lissajous figure analysis. If a Lissajous figure is desired, the output of the oscillator is also coupled to the horizontal plates of the oscilloscope. If temperature-dependent data are desired, a suitable furnace or cryogenic chamber is used. Details of the equipment are as follows:

7.2 *Audio Oscillator*, having a continuously variable frequency output from about 100 Hz to at least 30 kHz. Frequency drift shall not exceed 1 Hz/min for any given setting.

7.3 *Audio Amplifier*, having a power output sufficient to ensure that the type of transducer used can excite any specimen the mass of which falls within a specified range.

7.4 *Transducers*—Two are required; one used as a driver may be a speaker of the tweeter type or a magnetic cutting head or other similar device depending on the type of coupling chosen for use between the transducer and the specimen. The other transducer, used as a detector, may be a crystal or magnetic reluctance type of photograph cartridge. A capacitive pickup may be used if desired. An electromagnetic coupling system with an attached metal foil may also be used, with due consideration for effects of the foil on the natural vibration of the test bar. The frequency response of the transducer across the frequency range of interest shall have at least a 6.5 kHz bandwidth before  $-3$  dB power loss occurs.

7.5 *Power Amplifier*, in the detector circuit shall be impedance matched with the type of detector transducer selected and shall serve as a prescope amplifier.

7.6 *Cathode-Ray Oscilloscope*, any model suitable for general laboratory work.

7.7 *Frequency Counter*, preferably digital, shall be able to measure frequencies to within  $\pm 1$  Hz.

7.8 *Furnace*—If data at elevated temperature are desired, a furnace shall be used that is capable of controlled heating and

cooling. It shall have a specimen zone large enough for the specimen to be uniform in temperature within  $\pm 5^{\circ}\text{C}$  along its length through the range of temperatures encountered in testing. It is recommended that an independent thermocouple be placed in close proximity to (within 5 mm), but not touching, the center of the specimen to accurately measure temperature during heating and cooling.

7.9 *Cryogenic Chamber*—For data at cryogenic temperatures, any chamber shall suffice that shall be capable of controlled heating/cooling, frost-free and uniform in temperature within  $\pm 5^{\circ}\text{C}$  over the length of the specimen at any selected temperature. A suitable cryogenic chamber is shown in Fig. 2 (2). It is recommended that an independent thermocouple be placed in close proximity to (within 5 mm), but not touching, the center of the specimen to accurately measure temperature during heating and cooling.

7.10 *Specimen Suspension*—Any method of specimen suspension shall be used that is adequate for the temperatures encountered in testing and that allows the specimen to vibrate without significant restriction. Thread suspension is the system of choice for cryogenic and high-temperature testing. (See Fig. 1 and Fig. 3.) Common cotton thread, silica-glass fiber thread, oxidation-resistant nickel (or platinum) alloy wire, or platinum wire may be used. If metal wire suspension is used in the furnace, coupling characteristics will be improved if, outside the temperature zone, the wire is coupled to cotton thread, and the thread is coupled to the transducer. The specimen should be initially suspended at distances of approximately  $0.1 L$  from each end. The specimen should not be suspended at its fundamental flexural node locations ( $0.224 L$  from each end). The suspension point distances can be adjusted experimentally to maximize the vibrational deflection and resulting signal. For torsional vibration, the axes of suspension have to be off-center from the longitudinal axis of the specimen (shown in Fig. 3).

7.11 *Specimen Supports*—If the specimen is supported on

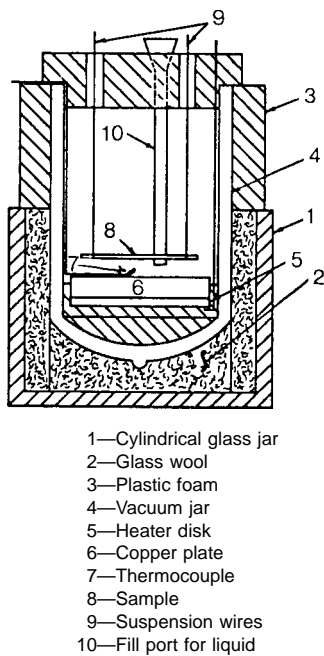


FIG. 2 Detail Drawing of a Typical Cryogenic Chamber

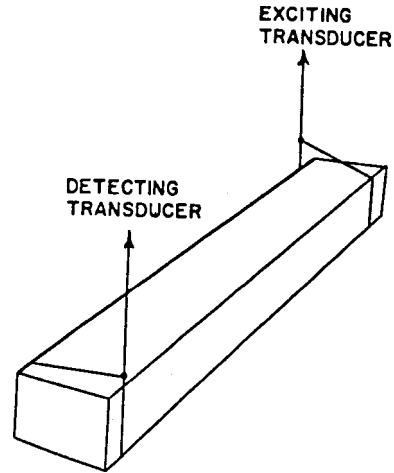


FIG. 3 Specimen Positioned for Measurement of Flexural and Torsional Resonant Frequencies Using Thread or Wire Suspension

direct contact supports, the supports shall permit the specimen to oscillate without significant restriction in the desired mode. This is accomplished for flexural modes by supporting the specimen at its transverse fundamental node locations ( $0.224 L$  from each end). In torsional modes the specimen should be supported at its center point. The supports should have minimal area in contact with the specimen and shall be cork, rubber, or similar material. In order to properly identify resonant frequencies, the transducers should be movable along the total specimen length and width. (See Fig. 4.) The transducer contact pressure should be consistent with good response and minimal interference with the free vibration of the specimen.

8. Test Specimen

8.1 Prepare the specimens so that they are either rectangular or circular in cross section. Either geometry can be used to measure both dynamic Young's modulus and dynamic shear modulus. However, experimental difficulties in obtaining torsional resonant frequencies for a cylindrical specimen usually preclude its use in determining shear modulus, although the equations for computing shear modulus with a cylindrical specimen are both simpler and more accurate than those used with a rectangular bar.

8.2 Resonant frequencies for a given specimen are functions of the bar dimensions as well as its mass and moduli; therefore,

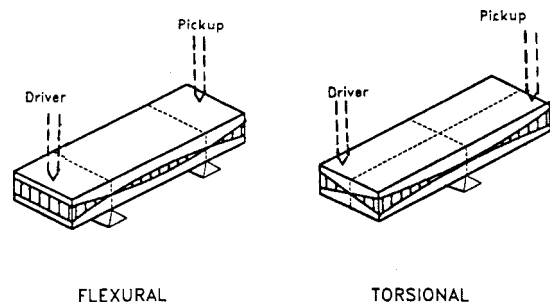


FIG. 4 Specimen Positioned for Measurement of Flexural and Torsional Resonant Frequencies Using Direct Support and Direct Contact Transducers



dimensions should be selected with this relationship in mind. Make selection of size so that, for an estimated modulus, the resonant frequencies measured will fall within the range of frequency response of the transducers used. A slender rod with a ratio of length to minimum cross-sectional dimension greater than ten and approximately 25 is preferred for ease in calculation. For shear modulus measurements of rectangular bars, a ratio of width to thickness of five is recommended for minimizing experimental difficulties. Suitable rectangular specimen dimensions are: 75 mm in length, 15 mm in width, and 3 mm in thickness. Suitable cylindrical rod dimensions are: 125 mm in length and 6 mm in diameter.

8.2.1 These specimen sizes should produce a fundamental flexural resonant frequency in the range from 1000 to 10 000 Hz and a fundamental torsional resonant frequency in the range from 10 000 to 30 000 Hz. (Representative values of Young's modulus are 410 GPa ( $59 \times 10^6$  psi) for alumina (99 %), 200 GPa ( $29 \times 10^6$  psi) for silicon nitride, and 530 GPa ( $77 \times 10^6$  psi) for titanium diboride.) Specimens shall have a minimum mass of 5 g to avoid coupling effects; any size of specimen that has a suitable length-to-cross section ratio in terms of frequency response and meets the mass minimum may be used. Maximum specimen size and mass are determined primarily by the power of the test system and physical space capabilities.

8.3 Finish the surfaces of the specimen using a fine grind (400 grit or finer). All surfaces on the rectangular specimen shall be flat. Opposite surfaces across the length and width shall be parallel within 0.01 mm or  $\pm 0.1\%$  whichever is greater. Opposite surfaces across the thickness shall be parallel within 0.002 mm or  $\pm 0.1\%$  whichever is greater. The cylindrical specimen shall be round and constant in diameter within 0.002 mm or  $\pm 0.1\%$  whichever is greater.

8.4 Dry the specimen in air at 120°C in a drying oven until the mass is constant (less than 0.1 % or 10 mg difference in mass with 30 min of additional drying).

**9. Procedure**

*9.1 Procedure A—Room-Temperature Testing:*

9.1.1 Switch on all electrical equipment and allow to stabilize in accordance with the manufacturer's recommendations. Suspend or support the specimen properly (see Fig. 3 and Fig. 4). Activate the equipment so that power adequate to excite the specimen is delivered to the driving transducer. Set the gain of the detector circuit high enough to detect vibration in the specimen and to display it on the oscilloscope screen with sufficient amplitude to measure accurately the frequency at which the signal amplitude is maximized. Adjust the oscilloscope so that a sharply defined horizontal baseline exists when the specimen is not excited. Scan frequencies with the audio oscillator until specimen resonance is indicated by a sinusoidal pattern of maximum amplitude on the oscilloscope or by a single closed loop Lissajous pattern. (It is recommended that the frequency scan start at a low frequency and then increase.) To verify that the frequency is fundamental and not an overtone, either the node/anti-node locations or one or more overtones should be identified (see Note 1). If a determination of the shear modulus is made, offset the coupling to the transducers so that the torsional mode of vibration may be induced and detected. (See Fig. 3 and Fig. 4.)

NOTE 1—The proper identification of the fundamental flexural mode is important as spurious frequencies inherent in the system may interfere, especially when greater excitation power and detection sensitivity are required for work with a specimen that has a poor response. The location of the nodes for the fundamental and the first four overtones are indicated in Fig. 5. One method to locate the nodes on the specimen is to move the detector along the length of the specimen; a node is indicated when the output amplitude goes to zero. An anti-node is indicated when the output amplitude reaches a local maximum. Another node location method (used often with string suspensions) is to lay a thin rod across the specimen at a presumed node or anti-node location. If the output amplitude is not affected, then the rod is on a node; if the output amplitude goes to zero, then the location is an anti-node. When several resonant flexural frequencies have been identified, the lowest frequency can be verified as the fundamental, if the numerical ratios of the first three overtone frequencies to the lowest frequency are: 2.7, 5.4, and 8.9. Note that these ratios are for a Bernoulli-Euler (simple) beam under ideal conditions. Typically the ratios will be slightly lower.

9.1.2 Find and verify (see Note 2) the fundamental resonant frequency in the torsion mode. The dimensions and mass of the specimen may be measured before or after the test. Measure the length and width dimensions within  $\pm 0.01$  mm or  $\pm 0.1\%$  (whichever is greater) at three locations and determine the average for each dimension. Measure the thickness/diameter within  $\pm 0.002$  mm or  $\pm 0.1\%$  (whichever is greater) at three locations and determine the average of the three measurements. Measure the mass within  $\pm 10$  mg or  $\pm 0.1\%$  (whichever is greater).

NOTE 2—Identification of the fundamental torsional mode is based on the same approaches used in identifying the flexural modes; node identification or frequency ratios, or both. Fig. 5 locates the node positions for torsional vibrations. The ratios of the first three torsional overtones to the fundamental torsional frequency are 2, 3, and 4.

9.2 *Procedure B—Elevated-Temperature Testing*—Determine the mass, dimensions, and resonant frequencies at room temperature in air as outlined in 9.1. Place the specimen in the furnace and adjust the driver-detector system so that all the frequencies to be measured can be detected without further adjustment. Determine the resonant frequencies at room temperature in the furnace cavity with the furnace doors closed, etc., as will be the case at elevated temperatures. Heat the furnace at a controlled rate that does not exceed 150°C/h. Take data at 25° intervals or at 15 min intervals as dictated by heating rate and specimen composition. Follow the change in resonant frequencies with time and temperature closely to

HARMONIC	FLEXURAL	FRACTIONAL DISTANCE FROM END FOR EACH NODAL LOCATION
1F		0.224
2F		0.132, 0.500
3F		0.0944, 0.3558
4F		0.0733, 0.277, 0.500
5F		0.060, 0.224, 0.409
<b>TORSIONAL</b>		
1T		0.500
2T		0.250
3T		0.167, 0.500
4T		0.125, 0.375

FIG. 5 Dynamic Modulus Resonant Modes and Nodal Locations Tracking Guide Template

avoid losing the identity of each frequency. (The overtones in flexure and the fundamental in torsion may be difficult to differentiate if not followed closely; spurious frequencies inherent in the system may also appear at temperatures above 600°C using certain types of suspensions, particularly wire.) If desired, data may also be taken on cooling. It must be remembered, however, that high temperatures may alter the specimen either reversibly or permanently (for example, phase change, devitrification, or microcracking). Such potential changes should be considered in planning the range of test temperatures and in interpreting test results as a function of temperature. Dimensions and mass of the specimen should be measured both before and after the test to check for permanent thermal effects. Measurements should be made to the precision described in 9.1.

9.3 Procedure C—Cryogenic Testing—Determine the mass, dimensions, and resonant frequencies in air at room temperature, as outlined in 9.1. Measure the resonant frequencies at room temperature in the cryogenic chamber. Take the chamber to the minimum temperature desired (see Note 3), monitoring frequencies as the chamber is cooled. Allow the specimen to stabilize at minimum temperature for at least 15 min. Heating rate should not exceed 50°C/h and data may be taken at intervals of 10 min or 15°C or as desired. Dimensions and mass of the specimen should be measured both before and after the test to check for permanent thermal effects. Measurements should be made to the precision described in 9.1.

NOTE 3—**Caution:** Take care to remove water vapor from the chamber by flushing with dry nitrogen gas prior to chilling so that frost deposits on the specimen do not cause anomalous results.

10. Calculation

10.1 Dynamic Young’s Modulus (1,3)—For the fundamental in flexure of a rectangular bar calculate as follows (3):

$$E = 0.9465 (m f_f^2 / b) (L^3 / t^3) T_1 \tag{2}$$

where:

- $E$  = Young’s modulus, Pa,
- $m$  = mass of the bar, g, (see Note 4),
- $b$  = width of the bar, mm, (see Note 4),
- $L$  = length of the bar, mm, (see Note 4),
- $t$  = thickness of the bar, mm, (see Note 4),
- $f_f$  = fundamental resonant frequency of bar in flexure, Hz, and
- $T_1$  = correction factor for fundamental flexural mode to account for finite thickness of bar, Poisson’s ratio, etc.

and:

$$T_1 = 1 + 6.585 (1 + 0.0752 \mu + 0.8109 \mu^2)(t/L)^2 - 0.868 (t/L)^4 - \left[ \frac{8.340 (1 + 0.2023 \mu + 2.173 \mu^2)(t/L)^4}{1.000 + 6.338 (1 + 0.1408 \mu + 1.536 \mu^2)(t/L)^2} \right] \tag{3}$$

where:

$\mu$  = Poisson’s ratio.

NOTE 4—In the modulus equations the mass and length terms are given in units of grams and millimetres. However, the defined equations can also be used with mass and length terms in units of kilograms and metres with no changes in terms or exponents.

10.1.1 If  $L/t \geq 20$ , the  $T_1$  can be simplified to:

$$T_1 = [1.000 + 6.585 (t/L)^2] \tag{4}$$

and  $E$  can be calculated directly.

10.1.2 If  $L/t < 20$  and Poisson’s ratio is known, then  $T_1$  can be calculated directly from Eq. 3 and then used to calculate  $E$ .

10.1.3 If  $L/t < 20$  and Poisson’s ratio is not known, then an initial Poisson’s ratio must be assumed to start the computations. An iterative process is then used to determine a value of Poisson’s ratio, based on experimental Young’s modulus and shear modulus. The iterative process is flowcharted in Fig. 6 and described in 10.1.3.1 through 10.1.3.5 below.

10.1.3.1 Determine the fundamental flexural and torsional resonant frequency of the rectangular test specimen, as described in 9.1. Using Eq 8 and Eq 9, calculate the dynamic shear modulus of the test specimen for the fundamental torsional resonant frequency and the dimensions and mass of the specimen.

10.1.3.2 Using Eq 2 and Eqs. 3, calculate the dynamic Young’s modulus of the rectangular test specimen from the fundamental flexural resonant frequency, the dimensions, and mass of the specimen and the initial/iterative Poisson’s ratio. Care must be exercised in using consistent units for all the parameters throughout the computations.

10.1.3.3 The dynamic shear modulus and Young’s modulus values calculated in 10.1.3.1 and 10.1.3.2 are substituted into Eq 12 for Poisson’s ratio satisfying isotropic conditions. A new value for Poisson’s ratio is calculated for another iteration starting at 10.1.3.2.

10.1.3.4 The steps in 10.1.3.2 through 10.1.3.3 are repeated until no significant difference (2 % or less) is observed between the last iterative value and the final computed value of the Poisson’s ratio.

10.1.3.5 Self-consistent values for the moduli are thus obtained.

10.1.4 For the fundamental in flexure of a rod of circular cross section calculate as follows (3):

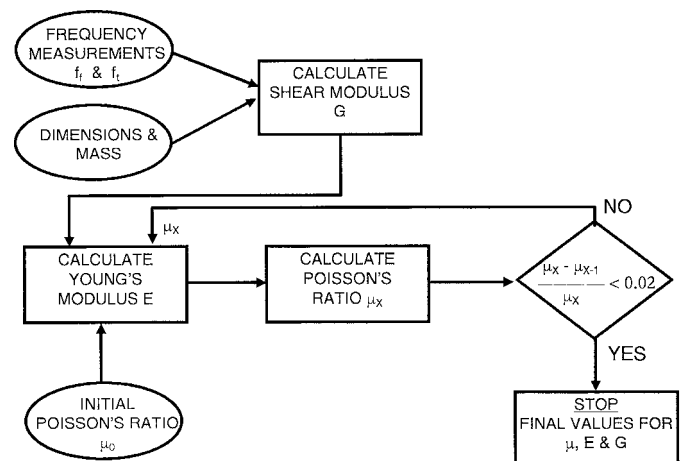


FIG. 6 Process Flowchart for Iterative Determination of Poisson’s Ratio

$$E = 1.6067 (L^3/D^4) (m f_f^2) T_1' \quad (5)$$

where:

$D$  = diameter of rod, mm, (see Note 4), and  
 $T_1'$  = correction factor for fundamental flexural mode to account for finite diameter of bar, Poisson's ratio, etc.

and

$$T_1' = 1 + 4.939(1 + 0.0752 \mu + 0.8109 \mu^2) (D/L)^2 - 0.4883 (D/L)^4 - \left[ \frac{4.691(1 + 0.2023 \mu + 2.173 \mu^2) (D/L)^4}{1.000 + 4.754(1 + 0.1408 \mu + 1.536 \mu^2) (D/L)^2} \right] \quad (6)$$

10.1.4.1 If  $L/D \geq 20$ , the  $T_1'$  can be simplified to the following:

$$T_1' = [1.000 + 4.939 (D/L)^2] \quad (7)$$

10.1.4.2 If  $L/D < 20$  and Poisson's ratio is known, then  $T_1'$  can be calculated directly from Eq 6 and then used to calculate  $E$ .

10.1.4.3 If  $L/D < 20$  and Poisson's ratio is not known, then an initial Poisson's ratio must be assumed to start the computations. Final values for Poisson's ratio, the dynamic Young's modulus, and dynamic shear modulus are determined, using the same method described in 10.1.3.1 through 10.1.3.5 and the modulus equations for circular bars (see Eq 5, Eq 6, and Eq 11).

10.2 Dynamic Shear Modulus (4) :

10.2.1 For the fundamental torsion of a rectangular bar calculate as follows. See Fig. 7 (4):

$$G = \frac{4 L m f_i^2}{b t} [ B / (1 + A) ] \quad (8)$$

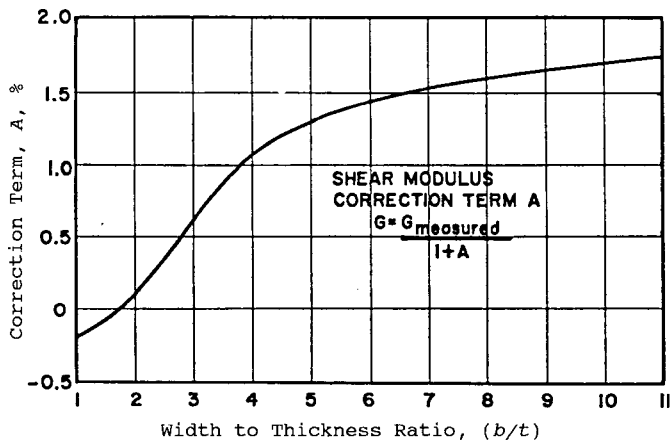


FIG. 7 Plot of the Shear Modulus Correction Term A

where:

$G$  = dynamic shear modulus, Pa,  
 $f_i$  = fundamental resonant frequency of bar in torsion, Hz,  
 $B = \frac{b/t + t/b}{4(t/b) - 2.52 (t/b)^2 + 0.21 (t/b)^6}$ , and (9)

$A$  = an empirical correction factor dependent on the width-to-thickness ratio of the test specimen (Ref (5)). This correction factor has an effect of less than 2 % and can be omitted, unless accuracies of better than 2 % are desired. (See Fig. 7 for a plot of  $A$  as a function of the width-to-thickness ratio.) A rational equation fitted to the points from Fig. 7 is given in Eq 10.

$$A = \frac{[0.5062 - 0.8776 (b/t) + 0.3504 (b/t)^2 - 0.0078 (b/t)^3]}{[12.03 (b/t) + 9.892 (b/t)^2]} \quad (10)$$

10.2.2 For the fundamental torsion of a cylindrical rod calculate as follows:

$$G = 16 m f_i^2 (L/\pi D^2) \quad (11)$$

10.3 Calculate Poisson's ratio as follows:

$$\mu = (E/2G) - 1 \quad (12)$$

where:

$\mu$  = Poisson's ratio,  
 $E$  = Young's modulus, and  
 $G$  = shear modulus.

10.4 Calculate moduli at elevated and cryogenic temperatures as follows:

$$M_T = M_o [f_T/f_o]^2 [1/(1 + \alpha \Delta T)] \quad (13)$$

where:

$M_T$  = modulus at temperature  $T$  (either Young's modulus,  $E$ , or shear modulus,  $G$ ),  
 $M_o$  = modulus at room temperature (either Young's modulus,  $E$ , or shear modulus,  $G$ ),  
 $f_T$  = resonant frequency in furnace or cryogenic chamber at temperature  $T$ ,  
 $f_o$  = resonant frequency at room temperature in furnace or cryogenic chamber,  
 $\alpha$  = average linear thermal expansion (mm/mm·°C) from room temperature to test temperature; (the method in Test Method C 372 is recommended), and  
 $\Delta T$  = temperature differential in °C between the test temperature  $T$  and room temperature.

10.5 Use the following stress conversion factor:

$$1 \text{ Pa} = 1.450 \times 10^{-4} \text{ psi} \quad (14)$$

11. Report

11.1 Report the following information:

11.1.1 Identification of specific tests performed and apparatus used, with a description of any deviations from the described practice.

11.1.2 Complete description of material(s) tested stating composition, number of specimens, specimen geometry and mass, specimen history, and any treatments to which the specimens have been subjected. Comments on surface finish, edge conditions, observed changes after cryogenic or high-temperature testing, etc. shall be included where pertinent.

11.1.3 Name of the person performing the test and date of the test.

11.1.4 Laboratory notebook number and page on which test data are recorded or the computer data file name, if used, or both.

11.1.5 Numerical values obtained for measured resonant frequencies, the dynamic Young's modulus, dynamic shear modulus, Poisson's ratio, and temperature of measurement for each specimen tested.

## 12. Precision and Bias

12.1 An intralaboratory study by Dickson and Wachtman (6) on 40 high-density alumina specimens demonstrated an uncertainty of 0.2 % for the dynamic shear modulus and 0.4 % for dynamic Young's modulus. The uncertainty included both random and systematic errors. This estimate was based upon uncertainties of 0.1 % on the thickness, width, and mass

measurements; an estimate of 0.1 % on the equations; and measurements of torsional frequency to 0.0007 % and of flexural frequency to 0.0015 %. The latter uncertainties were based upon frequency uncertainties of 0.08 Hz in torsion and 0.03 Hz in flexure. If frequencies are measured to an accuracy of 1 Hz, the uncertainty for frequency would be larger, but only 0.05 % in flexural and 0.01 % in torsion.

12.2 Spinner and Tefft (1) report that the measured frequencies of bulkier specimens are least affected by the method of coupling or the position of the supports with respect to the nodes. In view of these considerations a conservative generic estimate of the bias for resonant frequencies is about 1 part in 4000 for flexural resonance. For torsional resonant frequencies Spinner and Valore (5) estimate the bias as one part in 2000 for flat specimens and one part in 10 000 for square specimens.

12.3 A propagation of errors analysis of the equations for  $E$  and  $G$  using the stated precisions for dimensions, mass, and frequency measurements in this test method is in progress.

## 13. Keywords

13.1 advanced ceramics; dynamic; elastic modulus; elastic properties; Poisson's ratio; resonance; resonant beam; shear modulus; Young's modulus

## REFERENCES

- (1) Spinner, S., and Tefft, W. E., "A Method for Determining Mechanical Resonance Frequencies and for Calculating Elastic Moduli from These Frequencies," *Proceedings*, ASTM, 1961, pp. 1221–1238.
- (2) Smith, R. E., and Hagy, H. E., "A Low Temperature Sonic Resonance Apparatus for Determining Elastic Properties of Solids," *Internal Report 2195*, Corning Glass Works, April, 1961.
- (3) Spinner, S., Reichard, T. W., and Tefft, W. E., "A Comparison of Experimental and Theoretical Relations Between Young's Modulus and the Flexural and Longitudinal Resonance Frequencies of Uniform Bars," *Journal of Research of the National Bureau of Standards—A. Physics and Chemistry*, Vol 64A, No. 2, March–April, 1960.
- (4) Pickett, G., "Equations for Computing Elastic Constants from Flexural and Torsional Resonant Frequencies of Vibration of Prisms and Cylinders," *Proceedings*, ASTM, Vol 45, 1945, pp. 846–865.
- (5) Spinner, S., and Valore, R. C., "Comparisons Between the Shear Modulus and Torsional Resonance Frequencies for Bars and Rectangular Cross Sections," *Journal of Research*, National Bureau of Standards, Vol 60, 1958, RP2861, p. 459.
- (6) Dickson, R. W., and Wachtman, J. B., "An Alumina Standard Reference Material for Resonance Frequency and Dynamic Elastic Moduli Measurement I. For Use at 25°C," *Journal of Research of the National Bureau of Standards—A. Physics and Chemistry*, Vol 75A, No. 3, May–June, 1971, pp. 155–162.

*The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org).*