



Standard Test Method for Measuring Heat-Transfer Rate Using a Thermal Capacitance (Slug) Calorimeter¹

This standard is issued under the fixed designation E 457; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method describes the measurement of heat transfer rate using a thermal capacitance-type calorimeter which assumes one-dimensional heat conduction into a cylindrical piece of material (slug) with known physical properties.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.3 The values stated in SI units are to be regarded as the standard.

NOTE 1—For information see Test Methods E 285, E 422, E 458, E 459, and E 511.

2. Referenced Documents

2.1 ASTM Standards:

E 285 Test Method for Oxyacetylene Ablation Testing of Thermal Insulation Materials²

E 422 Test Method for Measuring Heat Flux Using a Water-Cooled Calorimeter²

E 458 Test Method for Heat of Ablation²

E 459 Test Method for Measuring Heat Transfer Rate Using a Thin-Skin Calorimeter²

E 511 Test Method for Measuring Heat Flux Using a Copper-Constantan Circular Foil, Heat-Flux Gage²

3. Summary of Test Method

3.1 The measurement of heat transfer rate to a slug or thermal capacitance type calorimeter may be determined from the following data:

3.1.1 Density and specific heat of the slug material,

3.1.2 Length or axial distance from the front face of the cylindrical slug to the back-face thermocouple,

3.1.3 Slope of the temperature—time curve generated by the back-face thermocouple, and

3.1.4 Calorimeter temperature history.

3.2 The heat transfer rate is thus determined numerically by

multiplying the density, specific heat, and length of the slug by the slope of the temperature–time curve obtained by the data acquisition system (see Eq 1).

3.3 The technique for measuring heat transfer rate by the thermal capacitance method is illustrated schematically in Fig. 1. The apparatus shown is a typical slug calorimeter which, for example, can be used to determine both stagnation region heat transfer rate and side-wall or afterbody heat transfer rate values. The annular insulator serves the purpose of minimizing heat transfer to or from the body of the calorimeter, thus approximating one-dimensional heat flow. The body of the calorimeter is configured to establish flow and should have the same size and shape as that used for ablation models or test specimens.

3.3.1 For the control volume specified in this test method, a thermal energy balance during the period of initial linear temperature response can be stated as follows:

$$\text{Energy Received by the Calorimeter (front face)} \quad (1)$$

$$= \text{Energy Conducted Axially Into the Slug}$$

$$q_c = \rho C_p l (\Delta T / \Delta \tau) = (M C_p / A) (\Delta T / \Delta \tau)$$

where:

\dot{q}_c = calorimeter heat transfer rate, W/m^2 ,

ρ = density of slug material, kg/m^3 ,

C_p = average specific heat of slug material during the temperature rise (ΔT), $\text{J/kg}\cdot\text{K}$,

l = length or axial distance from front face of slug to the thermocouple location (back-face), m ,

ΔT = $(T_f - T_i)$ = calorimeter slug temperature rise during exposure to heat source (linear part of curve), K ,

$\Delta \tau$ = $(\tau_f - \tau_i)$ = time period corresponding to ΔT temperature rise, s ,

M = mass of the cylindrical slug, kg ,

A = cross-sectional area of slug, m^2 .

In order to determine the steady-state heat transfer rate with a thermal capacitance-type calorimeter, Eq 1 must be solved by using the known properties of the slug material³ (for example, density and specific heat)—the length of the slug, and the slope (linear portion) of the temperature–time curve obtained during

¹ This test method is under the jurisdiction of ASTM Committee E-21 on Space Simulation and Applications of Space Technology and is the direct responsibility of Subcommittee E21.08 on Thermal Protection.

Current edition approved Oct. 10, 1996. Published December 1996. Originally published as E 457 – 72. Last previous edition E 457 – 72 (1990) ϵ^1 .

² *Annual Book of ASTM Standards*, Vol 15.03.

³ “Thermophysical Properties of High Temperature Solid Materials,” TPRC, Purdue University, or “Handbook of Thermophysical Properties,” Tolukian and Goldsmith, MacMillan Press, 1961.

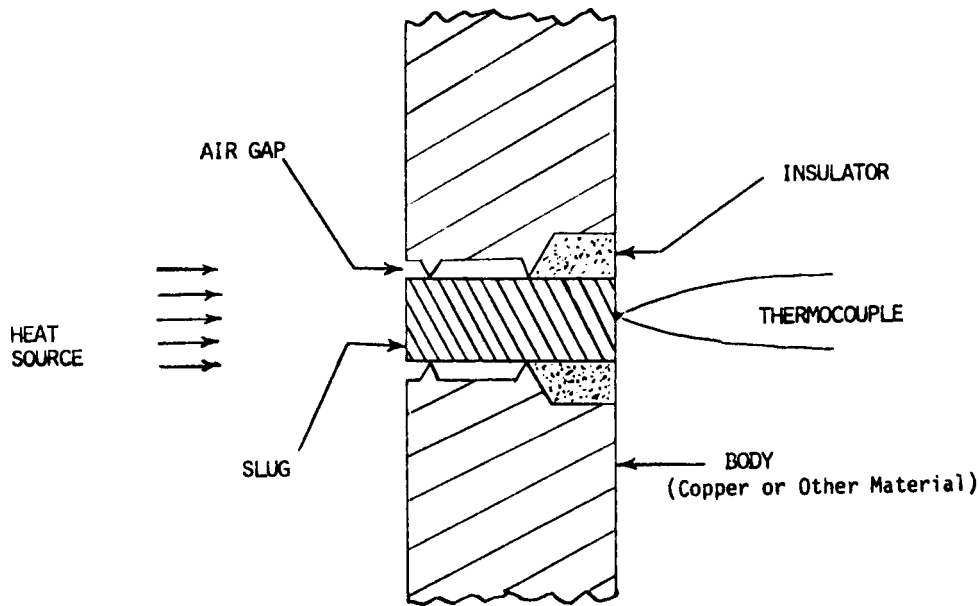


FIG. 1 Schematic of a Thermal Capacitance (Slug) Calorimeter

the exposure to a heat source. The initial and final temperature transient effects must be eliminated by using the initial linear portion of the curve (see Fig. 2).

3.3.2 In order to calculate the initial response time for a given slug, Eq 2 may be used.⁴

$$\tau_R = \frac{l^2 \rho C_p}{k \pi^2} \ln \left(\frac{2}{1 - \frac{q_{\text{indicated}}}{q_{\text{input}}}} \right) \quad (2)$$

where:

k = thermal conductivity of slug material, W/m·K

3.3.3 For maximum linear test time (temperature–time curve) within an allowed surface temperature limit, the relation shown as Eq 3 may be used for a calorimeter which is insulated by a gap at the back face.⁵

$$\tau_{\text{max,opt.}} = 0.48 \rho l C_p (\Delta T_{\text{front face}} / \dot{q}) \quad (3)$$

where:

$\Delta T_{\text{front face}}$ = the calorimeter final front face temperature minus the initial front face (ambient) temperature, T_o .

3.3.4 Eq 3 is based on the optimum length of the slug which can be obtained by applying Eq 4 as follows:

$$l_{\text{opt.}} = 3 k \Delta T_{\text{front face}} / 5 \dot{q}_c \quad (4)$$

3.4 To minimize side heating or side heat losses, the body is separated physically from the calorimeter slug by means of an insulating gap or a low thermal diffusivity material, or both. The insulating gap that is employed should be small, and recommended to be no more than 0.05 mm on the radius. Thus,

if severe pressure variations exist across the face of the calorimeter, side heating caused by flow into or out of the insulation gap would be minimized. Depending on the size of the calorimeter surface, variations in heat transfer rate may exist across the face of the calorimeter; therefore, the measured heat transfer rate represents an average heat transfer rate over the surface of the slug.

3.5 Since interpretation of the data obtained by this test method is not within the scope of this discussion, such effects as surface recombination and thermo-chemical boundary layer reactions are not considered in this test method.

3.6 If the thermal capacitance calorimeter is used to measure only radiative heat transfer rate or combined convective/radiative heat transfer rate values, the surface reflectivity of the calorimeter should be measured over the wavelength region of interest (depending on the source of radiant energy).

4. Significance and Use

4.1 The purpose of this test method is to measure the rate of thermal energy per unit area transferred into a known piece of material (slug) for purposes of calibrating the thermal environment into which test specimens are placed for evaluation. The calorimeter and holder size and shape should be identical to that of the test specimen. In this manner, the measured heat transfer rate to the calorimeter can be related to that experienced by the test specimen.

4.2 The slug calorimeter is one of many calorimeter concepts used to measure heat transfer rate. This type of calorimeter is simple to fabricate, inexpensive, and readily installed since it is not water-cooled. The primary disadvantages are its short lifetime and relatively long cool-down time after exposure to the thermal environment. In measuring the heat transfer rate to the calorimeter, accurate measurement of the rate of rise in back-face temperature is imperative.

4.3 In the evaluation of high-temperature materials, slug calorimeters are used to measure the heat transfer rate on

⁴ Ledford, R. L., Smotherman, W. E., and Kidd, C. T., "Recent Developments in Heat-Transfer Rate, Pressure, and Force Measurements for Hotshot Tunnels," AEDC-TR-66-228 (AD645764), January 1967.

⁵ Kirchhoff, R. H., "Calorimetric Heating-Rate Probe for Maximum-Response-Time Interval," *American Institute of Aeronautics and Astronautics Journal*, AIAA, Vol 2, No. 5, May 1964, pp. 966–67.

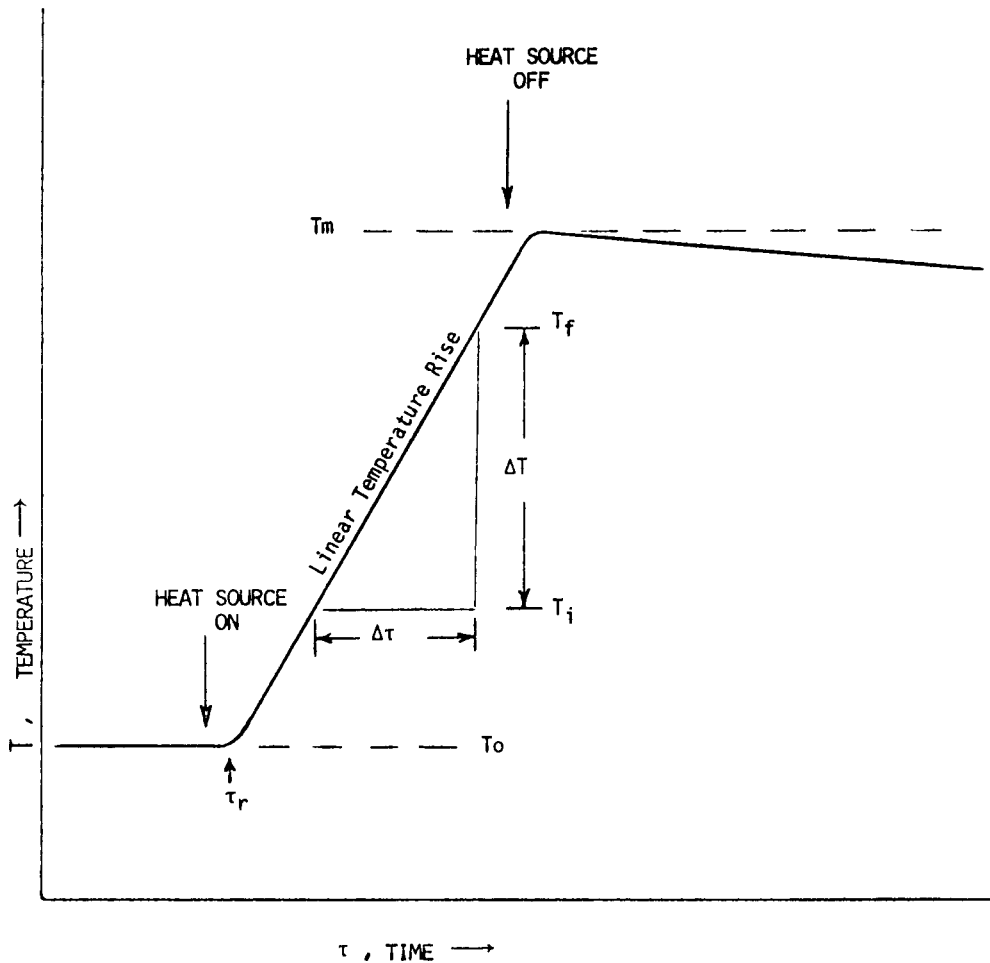


FIG. 2 Typical Temperature—Time Curve for Slug Calorimeter

various parts of the instrumented models, since heat transfer rate is one of the important parameters in evaluating the performance of ablative materials.

4.4 Regardless of the source of thermal energy to the calorimeter (radiative, convective, or a combination thereof) the measurement is averaged over the calorimeter surface. If a significant percentage of the total thermal energy is radiative, consideration should be given to the emissivity of the slug surface. If non-uniformities exist in the input energy, the heat transfer rate calorimeter would tend to average these variations; therefore, the size of the sensing element (that is, the slug) should be limited to small diameters in order to measure local heat transfer rate values. Where large ablative samples are to be tested, it is recommended that a number of calorimeters be incorporated in the body of the test specimen such that a heat transfer rate distribution across the heated surface can be determined. In this manner, more representative heat transfer rate values can be defined for the test specimen and thus enable more meaningful interpretation of the test. The slug selection may be determined using the nomogram as a guide (see Appendix X1).

5. Apparatus

5.1 *General*—The apparatus shall consist of a thermal capacitance (slug) calorimeter and the necessary instrumenta-

tion to measure the thermal energy transferred to the calorimeter. All calculations should use only those data taken after the heat source has achieved steady-state operating conditions. Wherever possible, it is desirable that several measurements be made of the required parameters.

5.2 *Back-Face Temperature Measurement*—The method of temperature measurement must be sufficiently sensitive and reliable to ensure accurate temperature rise data for the back-face thermocouple. Procedures should be adhered to in the calibration and preparation of the thermocouples. Attachment of the thermocouples should be such that the true back-side temperatures are obtained. Although no standardized procedures are available, methods such as resistance welding (small spot) and peening have been successfully used. The error in measurement of temperature difference between the initial and final times should not exceed $\pm 2\%$. The temperature measurements shall be recorded continuously using a commercially available recorder whose frequency response is at least ten times the expected frequency response of the slug to provide the accuracy required. During the course of operation of the plasma arc or other heat source, care must be taken to minimize deposits on the calorimeter surface.

5.3 *Data Acquisition*—The important parameter, back-face temperature rise, shall be automatically recorded throughout the calibration period. Recording speed will depend on the heat

transfer rate level such that the time range shall approach the temperature rise displacement on the recording paper. Timing marks shall be an integral part of the recorder output.

6. Procedure

6.1 It is essential that the thermal energy source (environment) be at steady-state conditions prior to testing if the thermal capacitance calorimeter is to produce representative heat transfer rate measurements. Make a millivolt scale calibration of the recorder prior to exposure of the calorimeter to the environment. With the recorder operating at the proper speed (see 4.3), expose the calorimeter to the thermal environment as rapidly as possible. After removal from the thermal environment, record the back-face temperature for sufficient time to determine the heat loss rate from the slug. Significant differences between the maximum and post-test values may indicate heat conduction losses to the calorimeter body. If feasible, obtain more than one measurement with more than one test method for a given thermal environment. To ensure that energy losses are minimized, the cooling rate slope should compare with the heating rate slope according to the following equation:

$$(\Delta T/\Delta \tau)_{\text{cooling}} \leq 0.05 (\Delta T/\Delta \tau)_{\text{heating}} \quad (5)$$

7. Heat Transfer Rate Calculation

7.1 The quantities as defined by Eq 1 shall be calculated

based on the physical properties of the slug material, dimensions of the slug, and the slope of the temperature–time curve of the calorimeter. The choice of units shall be consistent with the measured quantities. Variance analyses of thermal test conditions shall provide a sound basis for estimation of the reproducibility of the plasma arc or heat source environment. An error analysis of the measurements used in the heat transfer or energy determination is advisable.

8. Report

8.1 Report the following information:

- 8.1.1 Physical properties of the slug material,
- 8.1.2 Configuration of the calorimeter body,
- 8.1.3 Dimensions of the slug,
- 8.1.4 Slope of the temperature–time curve (linear portion), both heating and cooling histories, and
- 8.1.5 Calculated (apparent) corrected heat transfer rate (including losses).

9. Keywords

9.1 calorimeter; heat transfer rate; slug calorimeter; thermal capacitance

APPENDIX

(Nonmandatory Information)

X1. USE OF THE CALORIMETER SELECTION NOMOGRAM

X1.1 The calorimeter selection nomogram presented in this Appendix may be used to assist instrumentation personnel in choosing the appropriate calorimeter material, exposure time, front-face (surface) temperature rise for a given heat transfer rate, or any other combination of these parameters. This graphical method is intended as a guideline, not as a design criteria, and therefore should be used with an understanding of the basic test method for thermal capacitance (slug) calorimeters.

X1.2 The time from initial heat, τ , determined using the nomogram, will indicate the total exposure time, and not necessarily the optimum value. Average values of specific heat, C_p , thermal conductivity, k , and density, ρ , have been used in order to present a simple graphical representation of the basic equation below:

$$\tau = \pi(\rho k C_p) \left(\frac{\Delta T}{2 \dot{q} c} \right)^2 \quad (X1.1)$$

X1.3 For the slug to provide accurate results, the slope of the temperature–time curve must be obtained within the linear portion of the curve as defined by the following equation:

$$\dot{t}^2 [2(k/\rho C_p)] \leq \tau \leq 100 \dot{t}^2 / (k/\rho C_p) \quad (X1.2)$$

NOTE X1.1—The upper limit of the operating range is reduced by a factor of up to 100, if the calorimeter back face is in contact with a solid insulating material.

X1.4 To use the calorimeter selection nomogram (see Fig. X1.1), the known (or assumed) parameters must be noted on the appropriate scales (A, B, C, or D). A straight line must connect scales A and D, while another straight line connects scales B and C. The crossover line (without numbers) provides the pivot point for the two straight lines, as both must be coincident on the crossover line.

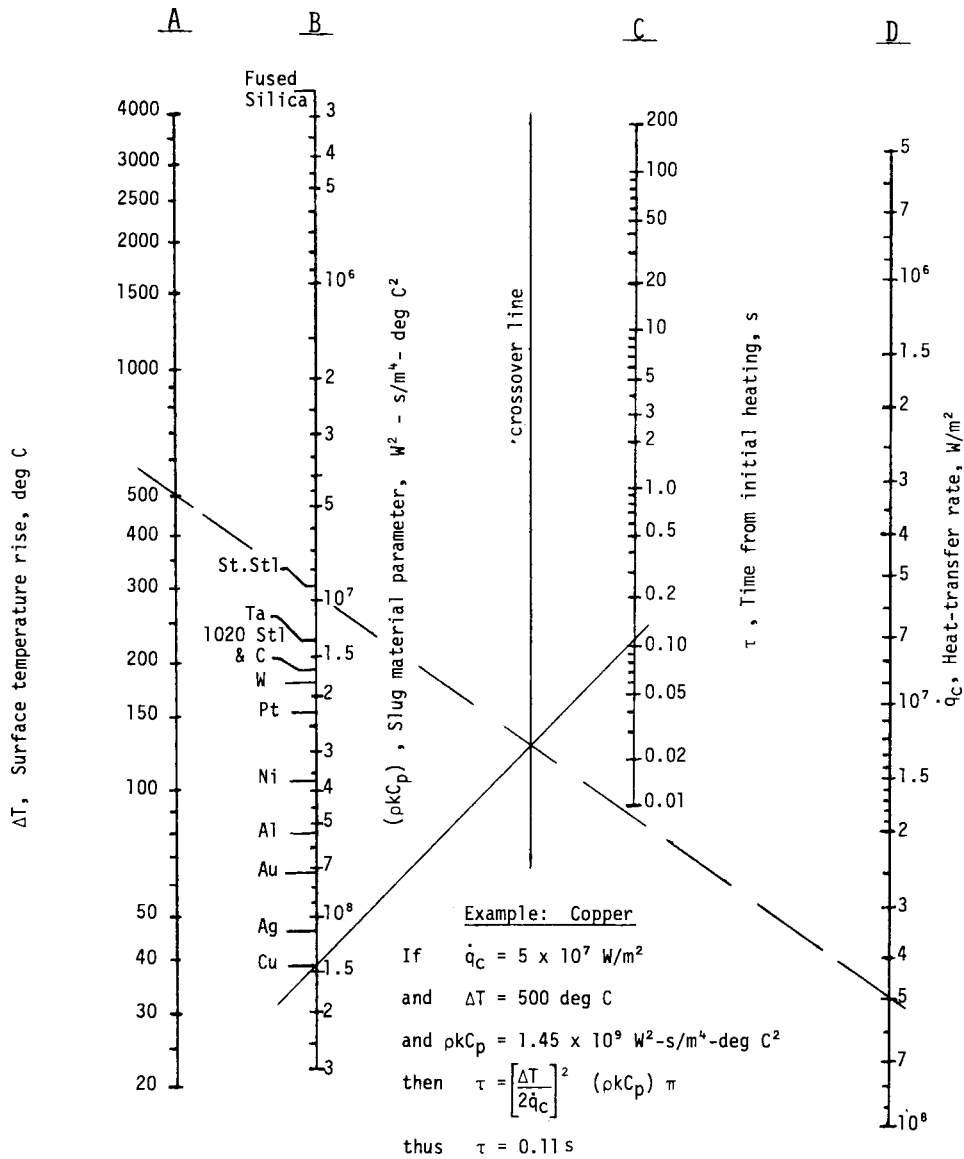


FIG. X1.1 Slug Selection Nomogram

The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, 100 Barr Harbor Drive, West Conshohocken, PA 19428.

This standard is copyrighted by ASTM, 100 Barr Harbor Drive, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (<http://www.astm.org>).